

## Article

# Development of Gas Sensor Array for Methane Reforming Process Monitoring

Dominik Dobrzyniewski <sup>1</sup> , Bartosz Szulczyński <sup>1</sup> , Tomasz Dymerski <sup>2,\*</sup>  and Jacek Gębicki <sup>1</sup> 

<sup>1</sup> Department of Process Engineering and Chemical Technology, Faculty of Chemistry, Gdańsk University of Technology, 11/12 G, Narutowicza Str., 80-233 Gdańsk, Poland; domdobrz@student.pg.edu.pl (D.D.); bartosz.szulczynski@pg.edu.pl (B.S.); jacebic@pg.edu.pl (J.G.)

<sup>2</sup> Department of Analytical Chemistry, Faculty of Chemistry, Gdańsk University of Technology, 11/12 G, Narutowicza Str., 80-233 Gdańsk, Poland

\* Correspondence: tomasz.dymerski@pg.edu.pl; Tel.: +48-58-348-6411

**Abstract:** The article presents a new method of monitoring and assessing the course of the dry methane reforming process with the use of a gas sensor array. Nine commercially available TGS chemical gas sensors were used to construct the array (seven metal oxide sensors and two electrochemical ones). Principal Component Regression (PCR) was used as a calibration method. The developed PCR models were used to determine the quantitative parameters of the methane reforming process: Inlet Molar Ratio (IMR) in the range 0.6–1.5, Outlet Molar Ratio (OMR) in the range 0.6–1.0, and Methane Conversion Level (MCL) in the range 80–95%. The tests were performed on model gas mixtures. The mean error in determining the IMR is 0.096 for the range of molar ratios 0.6–1.5. However, in the case of the process range (0.9–1.1), this error is 0.065, which is about 6.5% of the measured value. For the OMR, an average error of 0.008 was obtained (which gives about 0.8% of the measured value), while for the MCL, the average error was 0.8%. Obtained results are very promising. They show that the use of an array of non-selective chemical sensors together with an appropriately selected mathematical model can be used in the monitoring of commonly used industrial processes.

**Keywords:** gas sensors; sensor array; principal component regression; methane reforming; process monitoring



**Citation:** Dobrzyniewski, D.; Szulczyński, B.; Dymerski, T.; Gębicki, J. Development of Gas Sensor Array for Methane Reforming Process Monitoring. *Sensors* **2021**, *21*, 4983. <https://doi.org/10.3390/s21154983>

Academic Editor: Eduard Llobet

Received: 7 July 2021  
Accepted: 17 July 2021  
Published: 22 July 2021

**Publisher's Note:** MDPI stays neutral with regard to jurisdictional claims in published maps and institutional affiliations.



**Copyright:** © 2021 by the authors. Licensee MDPI, Basel, Switzerland. This article is an open access article distributed under the terms and conditions of the Creative Commons Attribution (CC BY) license (<https://creativecommons.org/licenses/by/4.0/>).

## 1. Introduction

The effects of carrying out all kinds of industrial processes are not always characterized by favorable influence on the environment. Increasingly stringent restrictions require industrial plants to constantly improve the analysis and process monitoring techniques. For this purpose, measurement techniques enabling quantitative and qualitative analysis are used, which focused mainly on the use of modern analytical techniques such as gas chromatography. The application of this type of method in an industrial plant carries the consequences of high investment costs and the necessity to provide appropriate infrastructure for the proper operation of the analyzers. In the case of gas samples, it is becoming more and more popular to design analyzers based on non-selective gas sensor arrays [1,2]. Matrices constructed in this way provide, among other things, a holistic analysis of the composition of the gas mixtures without separating them into individual components and shortening their duration. The most important advantage of this type of solution is the low price, which goes hand in hand with the simplicity of use. The latest applications of gas sensor arrays for the control and monitoring of industrial processes are presented in Table 1.

**Table 1.** Examples of the use of gas sensor arrays to monitor industrial processes.

| Sensor Array   | Number of Sensors | Process  | Reference |
|--|-------------------|--|-----------|
| An infrared matrix sensor  | 1                 | Monitor the FC stack temperature distribution  | [3]       |
| An array of thin film tin oxide sensors prepared by RF sputtering onto alumina and doped with chromium and indium  | 16                | Wine classification and prediction based on an electronic nose (e-nose)  | [4]       |
| Metal oxide semiconductors (MOSs) and Metal Oxide semiconductor field-effect transistors (MOSFETs)   | 50                | Monitors bioreactors and highlights their potential for controlling quality and safety, and for the optimization and automatic control of bioprocesses                     | [5]       |
| MOSFET-sensors with catalytic metal gates of palladium, iridium or platinum  | 10                | Non-invasive monitoring of the physiological changes in fermentation processes   | [6]       |
| Five TGS sensors from Figaro, Japan (TGS-832, TGS-823, TGS-2600, TGS-2610 and TGS-2611)  | 5                 | Predicting the optimum fermentation time at an earlier stage of the process  | [7]       |
| Sensor array of different types of metal oxide gas sensor (MOSs)   | 8                 | Study the tempeh fermentation process and the stages of this process   | [8]       |
| Sensor array was comprised of five sensors supplied by Figaro (Japan) and five sensors obtained from HANWIE Electronics (China)                              | 10                | Identification of different types of saffron, stigma of <i>Crocus sativus</i> , based on their volatile organic compounds (VOCs)   | [9]       |
| Semiconducting tin dioxide based sensors and an optical carbon detector  | 4                 | Monitoring an ethanol batch cultivation with the yeast <i>Saccharomyces cerevisiae</i>   | [10]      |
| Metal oxide sensor arrays  | 10                | Prediction of the alcohol content of the green jujube wine fermentation  | [11]      |
| Sensor array containing different gas-sensitive semiconductor devices and an infrared gas sensor   | 14                | Measuring the emission from a production-scale baker's yeast manufacturing process and monitor the gas emission from a yeast culture bioreactor during fed-batch operation | [12]      |
| Metal oxide sensor arrays  | 9                 | Determine the fermentation degree of cocoa beans   | [13]      |
| Metal oxide semiconductors (MOS) chemical sensors  | 18                | Identification of different fermentation times and bile species of <i>Bile Arisaema</i>  | [14]      |
| Potentiometric sensor array: polymeric cation-sensitive (8), polymeric anion-sensitive (8) and metallic and chalcogenide glass sensor with RedOx sensitivity | 23                | Real-time monitoring of ammonium and nitrate nitrogen in processed water at aeration plant   | [15]      |
| Hybrid sensor array composed by InterDigitated Chemocapacitor (IDVc) with the appropriate read-out electronic  | 8                 | The monitoring and evaluation and control of the specific Volatile Organic Compounds (VOCs)  | [16]      |

It should be objectively stated that all available analytical (instrumental) techniques will have smaller or larger defects affecting the quality of the analysis performed with their application. It is assumed that in order to develop an innovative and effective industrial processes monitoring system, a complementary and integrated approach, based on the synergy of their operation, is necessary [17,18]. Undoubtedly, this will ensure a full and comprehensive assessment of a given process sample, taking into account all possible factors, but on the other hand, many of these techniques have advantages that allow them to be used independently for specific tasks [19,20]. Table 2 shows the strengths and weaknesses of the use of sensor arrays for the analysis of process gas samples compared to the gas chromatography method.

Gas chromatography is widely used in the measurement, management, monitoring and control of processes carried out in breeding swine [21], municipal wastewater plants [22], municipal landfills [23] or even in the food industry, for example, in the production of cognac [24].

Recent research has been carried out intensively in the field of gas sensor arrays, as it has been observed that they can be used for continuous monitoring of industrial processes [25]. Due to the easily replaceable modules, it is possible to adapt the matrix to the current technological process, and the lack of selectivity of the sensors means that they are able to react to the presence of many substances belonging to the same group of chemical compounds, but each of them has a different sensitivity towards a given substance present in the sample [26]. It means that the principle of operation of the sensor arrays is the overlapping of the activity ranges of individual sensors, and the output signal is multidimensional and unique for a given gas mixture [20]. Such an approach requires the use of multivariate data analysis methods that allow the determination of desired


parameters of the sample on the basis of a multivariate set of signals from individual sensors of the matrix.

**Table 2.** Advantages and disadvantages of gas chromatography and sensor arrays.

| Analysis Method    | Advantages  | Disadvantages  |
|--------------------|---|--|
| Gas chromatography | <ul style="list-style-type: none"> <li>• Enables qualitative and quantitative analysis at the same time</li> <li>• High repeatability, reproducibility and accuracy</li> <li>• Possibility to identify all compounds present in the mixture</li> <li>• High resolution</li> </ul>                               | <ul style="list-style-type: none"> <li>• Limited measuring ranges and resulting from them a limit of quantification of individual compounds</li> <li>• Impossible to predict interactions between components</li> <li>• The necessity to store and transport of the samples</li> <li>• The representativeness and integrity of a sample depends on many factors</li> <li>• High costs</li> </ul> |
| Gas sensor arrays  | <ul style="list-style-type: none"> <li>• Enables continuous process monitoring</li> <li>• Sensor array in the form of easily replaceable modules</li> <li>• Uniqueness of the generated signal (a different signal for each tested mixture)</li> <li>• Low costs</li> <li>• Easy sensors calibration</li> </ul> | <ul style="list-style-type: none"> <li>• No qualitative analysis possible</li> <li>• High influence of temperature and humidity on measurement stability</li> <li>• Multidimensionality of the generated signal (requires averaging using statistical methods)</li> <li>• Complicates signal identification system (graphic methods, analytical procedures, neural network)</li> </ul>           |

This article presents the process of development of a sensor array to monitor the dry methane reforming process. Reforming is one of the methods of obtaining syngas (a gaseous mixture of hydrogen and carbon monoxide). Syngas is one of the basic products of the chemical industry, and at the same time, a raw material for many important processes. Therefore, the development of technologies allowing to minimize the carbon footprint of traditional methods of energy generation is undoubtedly one of the greatest challenges of science.

One type of methane reforming is DRM (dry methane reforming). The process proceeds according to the following reaction:



An important approach is to obtain a carbon monoxide and hydrogen mixture with a molar ratio of 1:1 by this reforming. Dry methane reforming is a promising alternative to the currently used processes leading to the production of syngas with a given ratio of hydrogen to carbon monoxide. The main advantage of dry reforming is the use of two main greenhouse gases as raw materials—methane and carbon dioxide. The dry reforming process is carried out at atmospheric pressure, which is also a great advantage in terms of safety and simplicity of the construction of the reactors. The composition of the synthesis gas obtained is suitable for the Fischer–Tropsch synthesis and alternative, clean fuels for diesel engines.

The article presents the development of a gas sensor array for process monitoring of the dry methane reforming process, based on commercially available chemical sensors. The article describes the selection of sensors used in the matrix and validation of the matrix with the use of model gas mixtures that reflect the composition of the process streams of the reforming process, so it can be used on an industrial scale to supervise and control the ongoing process in real-time to automate process analytics. The use of sensor arrays for process control has a very high application potential. It allows for a significant reduction in the cost of process control while maintaining the assumed accuracy of the obtained results.

## 2. Materials and Methods

### 2.1. Chemical Gas Sensors

For the presented research, a set of commercially available chemical gas sensors was selected. Figaro Engineering Inc. sensors from the TGS series were used. Basic information on the sensors used is presented in Table 3.

**Table 3.** Basic characteristics of Figaro Engineering Inc. gas sensors.

| Sensor Type               | Model   | Detected Gases                       |
|---------------------------|---------|--------------------------------------|
| Catalytic                 | TGS6810 | methane, propane, iso-butane         |
| Catalytic                 | TGS6812 | methane, propane, hydrogen           |
| Electrochemical           | TGS4161 | carbon dioxide                       |
| Electrochemical           | TGS5042 | carbon monoxide                      |
| Metal Oxide Semiconductor | TGS2600 | methane, carbon monoxide, hydrogen   |
| Metal Oxide Semiconductor | TGS2602 | hydrogen, toluene, ethanol           |
| Metal Oxide Semiconductor | TGS2603 | hydrogen, ethanol                    |
| Metal Oxide Semiconductor | TGS2611 | ethanol, hydrogen, methane           |
| Metal Oxide Semiconductor | TGS3870 | carbon monoxide, methane             |
| Metal Oxide Semiconductor | TGS823  | carbon monoxide, methane, iso-butane |
| Metal Oxide Semiconductor | TGS8100 | methane, hydrogen, ethanol           |

### 2.2. Gas Mixtures Preparation

All gas mixtures were prepared in Tedlar gas sampling bags. Three-liter bags were used, and the total volume of the prepared mixtures was 2000 mL each time. In order to prepare gas mixtures, the following steps had to be taken:

1. Assumption of the desired concentration of individual chemical substances in the gas mixture ( $C_m$ , ppm  $v/v$ ),
2. Assumption of the total volume of the gas mixture ( $V_m$ , mL),
3. Determination of the volume of individual substances that must be dosed into the Tedlar bag ( $V_i$ , mL):

$$V_i = \frac{C_m \cdot V_m}{10^6}, \quad (2)$$

4. Determination of the air volume ( $V_0$ , mL), which must be dosed into the Tedlar bag:

$$V_0 = V_m - \sum V_i, \quad (3)$$

The volume of air dosed to the Tedlar bag was controlled with a RED-Y GSC-B9SS-B23 mass flow controller. Individual chemicals were taken from gas cylinders containing pure gases (>99.9%, Linde Gaz Polska) and then dosed to the Tedlar bag using Hamilton gas-tight syringes.

To determine the correctness of making the mixtures, all prepared gas mixtures were analyzed using a gas chromatograph (AutoSystem XL, Perkin-Elmer, Norwalk, CT, USA) equipped with a Porapak Q column (Sigma-Aldrich, Merck, Darmstadt, Germany), 100–120 mesh, OD 3.2 mm  $\times$  6.5 m, and a thermal conductivity detector (TCD). The oven temperature was set at 60 °C. Turbochrom software was used for recording and processing of chromatograms.

### 2.3. Gas Sensor Array Measurements

The diagram of the test equipment constructed for the sensor analysis is shown in Figure 1. It consisted of the following elements: (1) Tedlar foil bag, (2) three-way valve, (3) air filter, (4) gas sensor array, (5) temperature sensor, (6) humidity sensor, (7) diaphragm pump, (8) pulse width modulation module, (9) analog-to-digital converter, (10) Arduino MEGA2560 platform, (11) computer. A stream of clean air flowed through the measuring chamber at a constant flow rate, controlled by the diaphragm pump rotation speed. The change in the pump rotation is caused by a change in the DC voltage supplied to the pump

motor. The PWM module (8) controlled by Arduino (10) is responsible for the regulation of the supply voltage. By changing the position of a three-way valve (2), a sample of the prepared gas mixture was directed to the measuring chamber. After completion of the measurement, clean air was returned to the measuring chamber in order to regenerate the sensors by changing the valve (2) position. Flushing the sensors with clean air made it possible to restore them to their initial parameters and prepare them for subsequent analyzes. The electrical systems for each of the sensors have been prepared in accordance with the manufacturer's requirements. The signals from the sensors were recorded using an analog-to-digital converter (ADS1015). All data were saved on the computer using dedicated software.

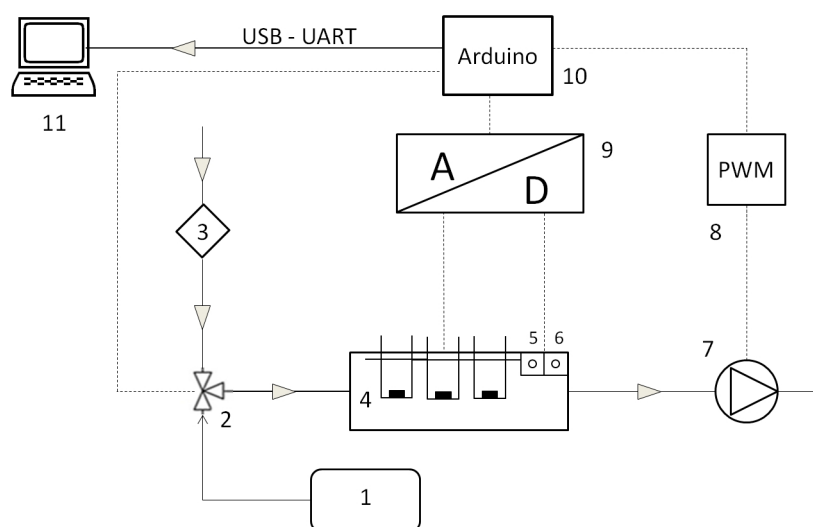


Figure 1. Gas sensor array testing system.

An example of the sensor response is shown in Figure 2. For data analysis, the relative sensor response ( $S_R$ ) was used. It was calculated using the formula:

$$S_R = \frac{\Delta S}{S_0} \quad (4)$$

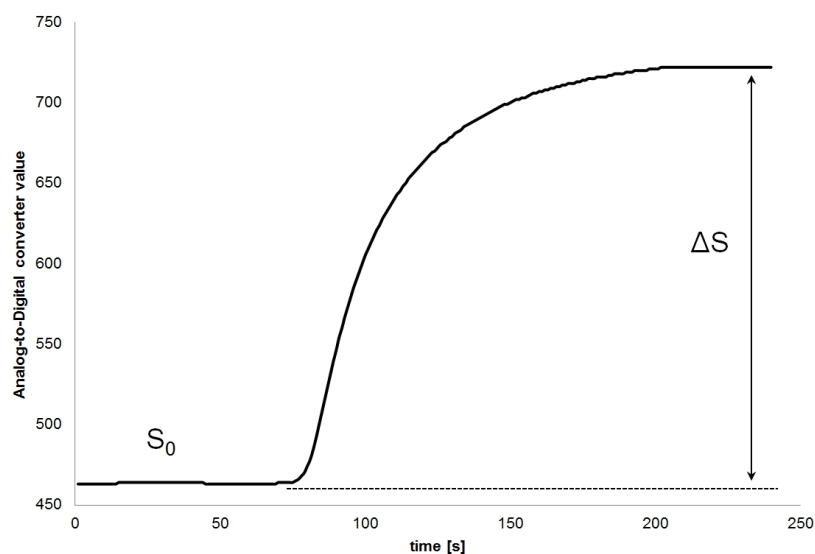


Figure 2. Example of the sensor response.

## 2.4. Data Analysis

Data analysis and other calculations were performed using RStudio Desktop (v. 1.0.143) software. Principal Component Regression (PCR) was selected as the calibration model for the gas sensor array. The PCR method tutorial in R language is presented on the website [27]. The chemical gas sensors are usually responsive to multiple gases, which would make them individually quite useless. For this reason, the PCR method was chosen as the data analysis method. It enables the deconvolution of the collected sensor data sets and minimizes the impact of low selectivity of sensors in the matrix. It should be noted that other methods of data analysis, such as Multiple Linear Regression (MLR) [28], Partial Least Squares Regression (PLSR) [29], or Artificial Neural Network (ANN) [30], can also be successfully used for this type of application.

This model assumes reducing the number of explanatory variables by selecting few first principal components (PCs) in the place of the primary variables. The guiding idea of the PCR method is to formulate a relationship between PCs and the expected concentration of the component. The method consists of two steps:

1. Determination of the principal components using the principal component analysis (PCA) method. It allows obtaining an uncorrelated matrix of variables.
2. Development of the Multiple Linear Regression (MLR) model with the use of principal components as variables.

A detailed representation of the PCR algorithm is presented in Figure 3.

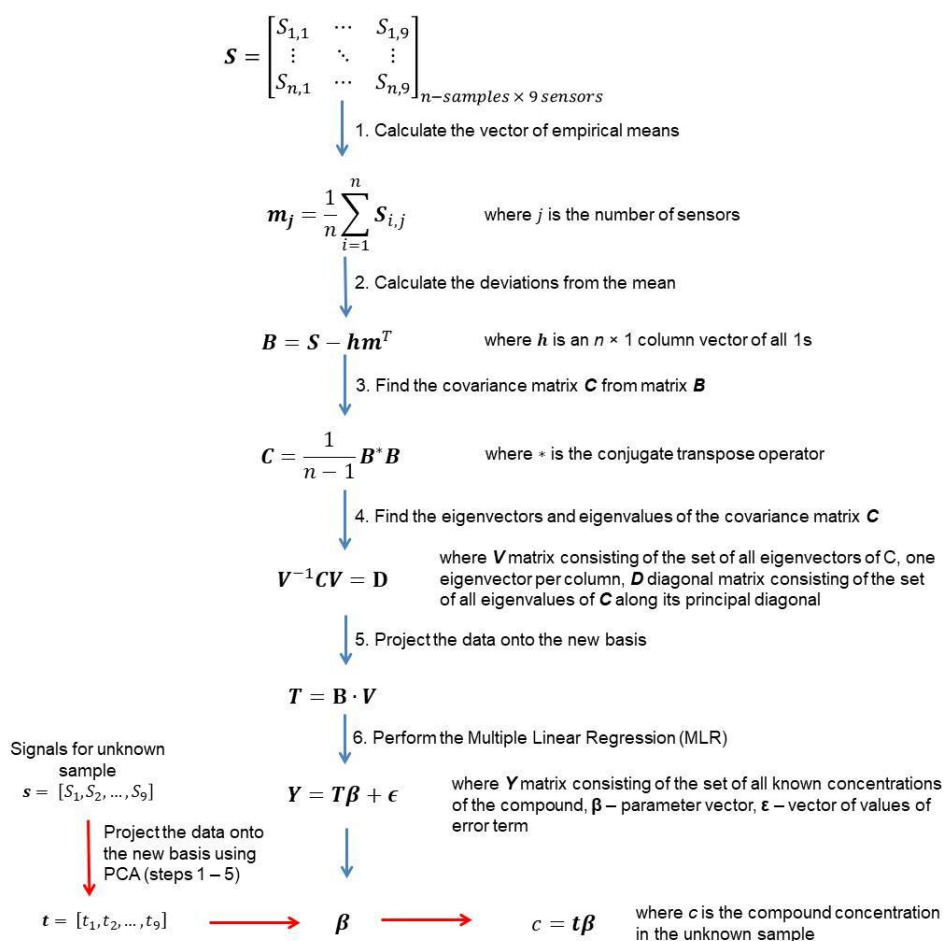


Figure 3. The PCR algorithm.



### 3. Results

In the first stage of the research, the static characteristics of all tested sensors were collected. For this purpose, mixtures of single compounds (methane, carbon dioxide, carbon monoxide and hydrogen) with air in the concentration range of 50–1000 ppm  $v/v$  were prepared. An example of the response characteristics to the presence of carbon monoxide determined for the TGS2600 sensor is shown in Figure 4. In order to ensure the linearity of the characteristics, they were plotted in the  $S = f(\log C)$  coordinates, where  $S$  is the signal obtained from the analog-to-digital converter, and  $C$  is the gas concentration in the mixture with air (ppm  $v/v$ ).

Based on the collected static characteristics, the sensitivity of each sensor to a single gas was determined. The values obtained are presented in Table 4.

Based on the obtained sensitivity values, a set of sensors for the matrix was selected. Only the catalytic sensors (TGS6810 and TGS6812) were rejected from the tested set due to the low sensitivity values in the tested concentration range. These sensors are used in the presence of high concentrations of explosive gases. Note that it is necessary to use electrochemical sensors TGS4161 and TGS5042, which show high sensitivity and selectivity towards carbon dioxide and carbon monoxide, respectively. The sensitivity values obtained for the remaining sensors indicate the correct selection of sensor models. All of them react to the presence of the tested gases.

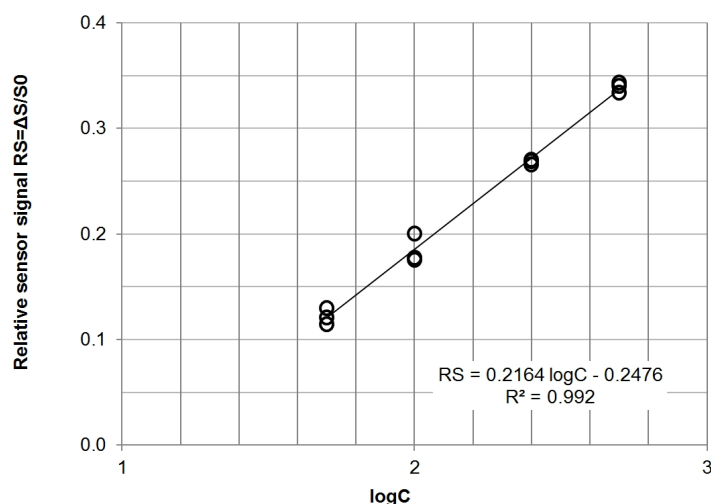


Figure 4. Static characteristics of the Figaro TGS2600 sensor in the presence of carbon monoxide.

Table 4. Sensitivity of the tested sensors.

|         | CH <sub>4</sub> | CO <sub>2</sub> | CO    | H <sub>2</sub> |
|---------|-----------------|-----------------|-------|----------------|
| TGS2600 | 0.114           | 0.034           | 0.216 | 0.332          |
| TGS2602 | 0.089           | 0.022           | 0.091 | 0.087          |
| TGS2603 | 0.082           | 0.025           | 0.085 | 0.221          |
| TGS2611 | 0.196           | 0.015           | 0.102 | 0.146          |
| TGS3870 | 0.165           | 0.012           | 0.033 | 0.074          |
| TGS4161 | 0.012           | 0.307           | 0.013 | 0.022          |
| TGS5042 | 0.019           | 0.009           | 0.247 | 0.042          |
| TGS6810 | 0.005           | 0.002           | 0.005 | 0.005          |
| TGS6812 | 0.004           | 0.001           | 0.006 | 0.005          |
| TGS823  | 0.211           | 0.019           | 0.233 | 0.185          |
| TGS8100 | 0.052           | 0.011           | 0.138 | 0.201          |


In the next step, model gas mixtures were prepared to reflect the expected inlet and outlet concentrations from the dry methane reforming process. The sensor matrix responses to all possible concentration combinations shown in Table 5 were recorded, repeating each

analysis three times. The DRM inlet stream is usually a pure mixture of methane and carbon dioxide; therefore, binary mixtures were used as inlet mixtures. In the case of outlet streams, the possible incomplete conversion of all substrates must be taken into account. Therefore, the outlet mixtures were prepared as four-component mixtures.

**Table 5.** Compositions of tested gas mixtures.

|                          | DRM Inlet Stream                    | DRM Outlet Stream     |
|--------------------------|-------------------------------------|-----------------------|
| total number of mixtures | 36                                  | 81                    |
| CH <sub>4</sub>          | 50, 100, 200, 300, 400, 500 ppm v/v | 10, 50, 100 ppm v/v   |
| CO <sub>2</sub>          | 50, 100, 200, 300, 400, 500 ppm v/v | 10, 50, 100 ppm v/v   |
| CO                       | -                                   | 100, 250, 500 ppm v/v |
| H <sub>2</sub>           | -                                   | 100, 250, 500 ppm v/v |

Based on the recorded matrix response signals, five PCR calibration models were developed: for the inlet stream (carbon dioxide and methane models) and for the outlet stream (carbon monoxide, hydrogen, and methane models). The validation of these models was performed on the basis of correlation charts presented in Figure 5.

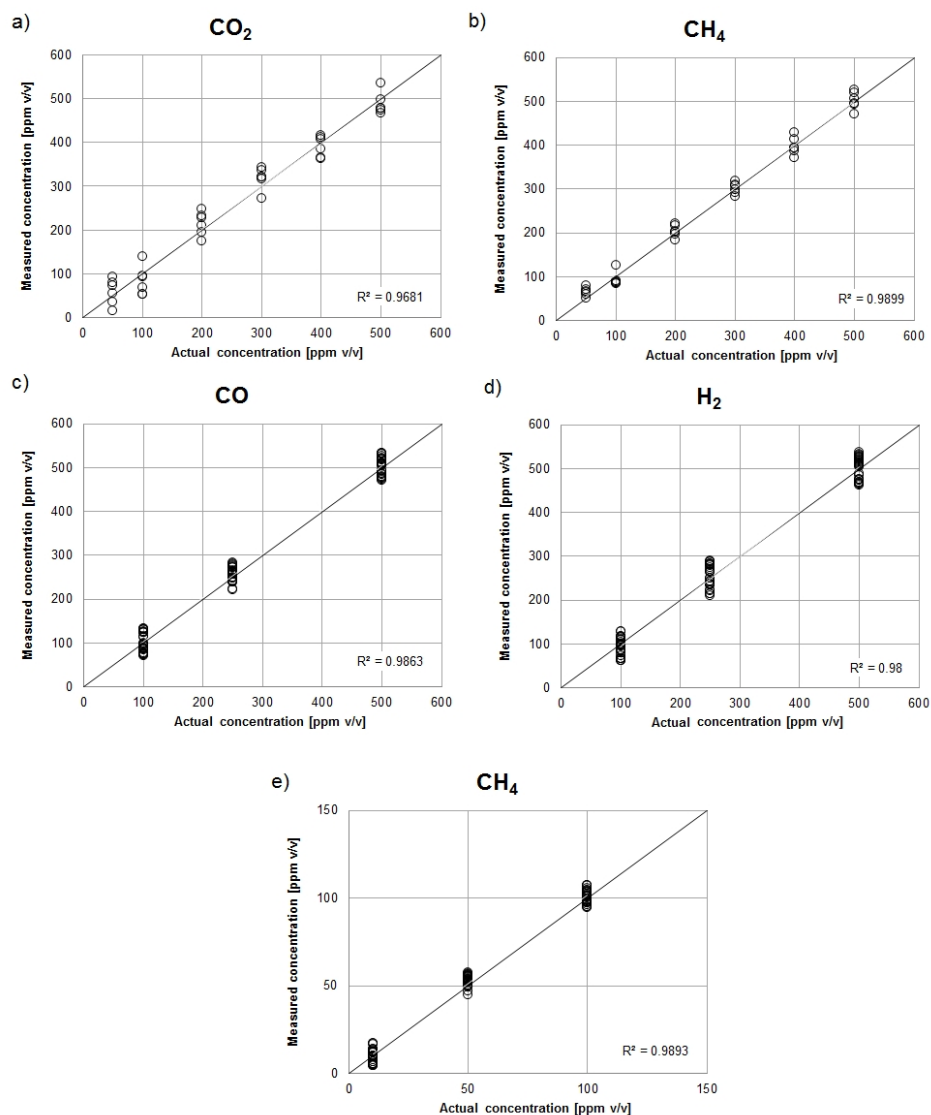

**Figure 5.** Validation plots of PCR calibration models for DRM inlet stream: (a) carbon dioxide, (b) methane and DRM outlet stream: (c) carbon monoxide, (d) hydrogen, (e) methane.



In the last stage of the research, gas mixtures simulating the actual compositions of process mixtures were prepared. The concentrations of individual components were determined using developed PCR models. The determined concentrations were converted into the following parameters characterizing the course of the dry methane reforming process:

1. Inlet molar ratio (IMR):

$$IMR = \frac{C_{CO_2}}{C_{CH_4}} \quad (5)$$

2. Outlet molar ratio (OMR):

$$OMR = \frac{C_{H_2}}{C_{CO}} \quad (6)$$

3. Methane conversion level (MCL):

$$MCL = \frac{C_{CH_4,in} - C_{CH_4,out}}{C_{CH_4,in}} \cdot 100\% \quad (7)$$

Figure 6 presents the IMR parameter determination using a gas sensor array in the range from 0.6 to 1.5. The Root-Mean-Square Error (RMSE) for the entire range is equal to 0.096. However, in the range 0.9–1.1, where these IMR values are most commonly found in industrial conditions, the RMSE is equal to 0.065.

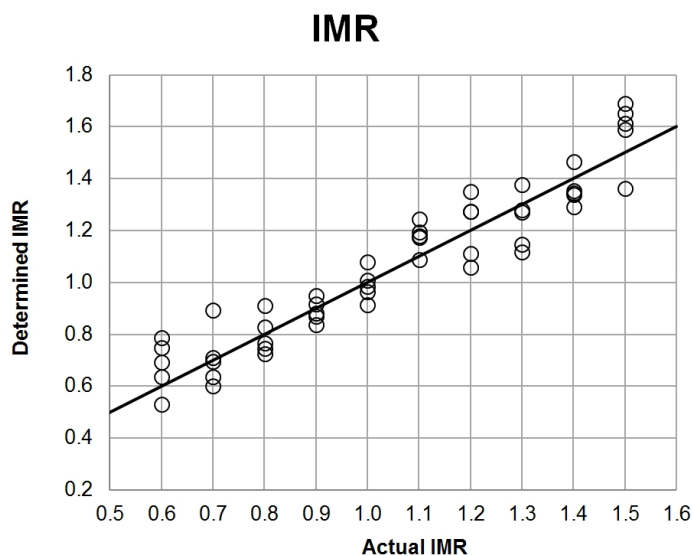


Figure 6. Actual and determined Inlet Molar Ratio (IMR) correlation plot.

Figure 7 presents the OMR and MCL values determined using a gas sensor array. They were measured using model gas mixtures, the composition of which was represented by the values of parameters equal to the intersections of the gridlines in Figure 7. Model gas mixtures with composition within the range of parameters: OMR 0.6–1.0 (step 0.5) and MCL 80–95% (step 5%) and 98% were used. The RMSE for MCL determination is equal to 0.8%, and for OMR determination, it is equal to 0.008.

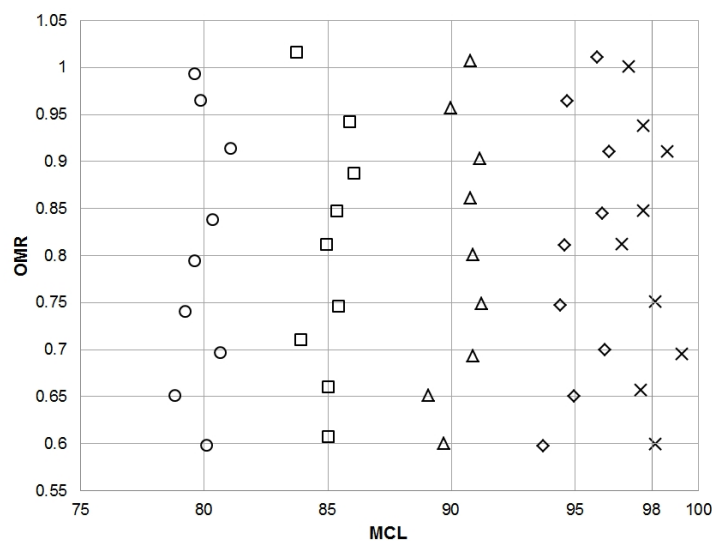


Figure 7. Actual and determined Inlet Molar Ratio (IMR) correlation plot.

#### 4. Discussion

The article presents a new method of monitoring and assessing the course of the dry methane reforming process with the use of a gas sensor array. Nine commercially available gaseous chemical sensors were used to construct the array. Such a solution enables the repeated production of the developed array, as opposed to solutions based on prototype sensors.

The performed tests of the sensitivity of sensors for the process mixtures components allowed to reject sensors that showed the lowest sensitivity in the assumed concentration range. These were the catalytic sensors TGS6810 and TGS6812. Two types of sensors were used in the final solution: electrochemical (2 pieces) and metal oxide sensors (7 pieces).

The array constructed in this way was calibrated to determine the concentrations of methane, carbon dioxide, carbon monoxide and hydrogen. Model gas mixtures representing the actual streams of the methane reforming process were used for calibration. Principal Component Regression (PCR) was used as a calibration method. The validity of the use of this method is confirmed by the values of the determination coefficients ( $R^2$ ) of the correlation plots (Figure 5), the value of which in all five cases was higher than 0.95.

The developed PCR models were used to determine the quantitative parameters of the description of the reforming process: Inlet Molar Ratio (IMR), Outlet Molar Ratio (OMR), and Methane Conversion Level (MCL). In the case of the input parameter (IMR), the mean error in determining this parameter is 0.096 for the range of molar ratios 0.6–1.5. However, in the case of the process range (0.9–1.1), this error is 0.065, which is about 6.5% of the measured value. The OMR and MCL values were determined for the mixtures representing outlet streams of the reforming process. For the molar ratio, an average error of 0.008 was obtained (which gives about 0.8% of the measured value), while for the conversion degree, the average error was 0.8%.

Such results are very promising. They show that the use of an array of non-selective chemical sensors together with an appropriately selected mathematical model can be used in the monitoring of commonly used industrial processes, such as, for example, methane reforming. However, it should be noted that these matrices cannot be used directly in the process stream. In the case of the presented research, all analyzes were carried out on model gas mixtures with component concentrations of up to about 1000 ppm  $v/v$  in air, under atmospheric pressure, at room temperature. In the actual reforming process, the streams have a temperature of 650–850 °C (in the case of dry reforming), and their composition is expressed in tens of percent. For this reason, the next step in future research should be to check the possibility of using the array in real conditions, using a sample cooler and a dilution module that would reduce gas concentrations to

the required ranges and also enable the operation of metal oxide semiconductor sensors, which require oxygen for proper operation. However, the cooling and dilution processes are basic operations that are performed in the case of process analytics; therefore, it can be assumed that the constructed array in this way can also be successfully used in real industrial conditions. An additional advantage is the low price of the sensors, compared to expensive chromatographic analyzers that require periodic maintenance and ensure the availability of high purity gases. According to the sensor manufacturer's declaration, their lifetime is about 2 years, which ensures a relatively long time of maintenance-free use.

The proposed solution can also be used to monitor biogas-fed processes. In such an application, the proposed matrix should be supplemented with sensors detecting hydrogen sulfide, ammonia, or nitrogen oxides. In this case, it is best to choose electrochemical sensors (for example, the Figaro FECS series) that allow the determination of these components at low concentration levels. The use of additional sensors requires additional calibrations using the PCR method, but thanks to this, it will also be possible to simultaneously monitor two processes—biogas purification and methane reforming.

In terms of the accuracy of the obtained results, the sensor matrices do not match the chromatographic methods, but in cases where the accuracy of the obtained results does not have to be high, they are a very good and, at the same time, cheap alternative to specialized instrumental techniques. The comparison of the constructed sensor matrix with commercially available solutions is presented in Table 6.

**Table 6.** The comparison of the constructed sensor matrix with commercially available devices.

| Producer   | Model  | Technology  | Range  | Accuracy  | Response Time                     | Reference |
|--|--|---|--|---|-----------------------------------|-----------|
| Gdańsk University of Technology                                | Sensor matrix prototype                          | MOS and EC gas sensors  | CO, CO <sub>2</sub> , CH <sub>4</sub> , H <sub>2</sub> : 0–100%<br>(using dilution system)<br>CO: 0–30%            | 5% Full Scale (FS)  | <90 s to 90% step range<br>(MOS)  | -         |
| Cubic Sensor and Instrument Co.                                | Portable Infrared Syngas Analyzer Gasboard-3100P | CO, CO <sub>2</sub> , CH <sub>4</sub> (NDIR)<br>H <sub>2</sub> (TCD)        | CO <sub>2</sub> : 0–25%<br>CH <sub>4</sub> : 0–10%<br>H <sub>2</sub> : 0–30%<br>CO: 0–30%                          | 2% Full Scale (FS)  | <15 s to 90% step range<br>(NDIR) | [31]      |
| Cubic Sensor and Instrument Co.                                | Syngas Analysis System Gasboard-9021             | CO, CO <sub>2</sub> , CH <sub>4</sub> (NDIR)<br>H <sub>2</sub> (TCD)        | CO <sub>2</sub> : 0–25%<br>CH <sub>4</sub> : 0–10%<br>H <sub>2</sub> : 0–30%                                       | CO, CO <sub>2</sub> , CH <sub>4</sub> < 1% FS<br>H <sub>2</sub> < 2% FS                             | <15 s to 90% step range<br>(NDIR) | [32]      |
| Hubei Cubic-Ruiyi Instrument CO.                               | Portable Natural Gas Analyzer Gasboard-3110P     | CO <sub>2</sub> , CH <sub>4</sub> (NDIR)                                    | CO <sub>2</sub> : 0–5%<br>CH <sub>4</sub> : 0–100%<br>CO: 0–2% or 0–50%  | <2% FS  | <15 s to 90% step range<br>(NDIR) | [33]      |
| Nova Analytical Systems (a Unit of Tenova Goodfellow Inc.)     | 970P Portable Multi-Gas Industrial Analyzers     | CO, CO <sub>2</sub> , CH <sub>4</sub> (NDIR)<br>H <sub>2</sub> (TCD)        | CO <sub>2</sub> : 0–2% or 0–50%<br>CH <sub>4</sub> : 0–2% or 0–50%<br>H <sub>2</sub> : 0–2% or 0–50%<br>CO: 0–100% | 0.1% for all gases<br><1% FS in 8 h   | 20–30 s to 90% step range         | [34]      |
| VASTHI Instruments Pvt Ltd.                                    | Online Syngas Analyzer by Vasthi                 | CO, CO <sub>2</sub> , CH <sub>4</sub> (NDIR)<br>H <sub>2</sub> (TCD)        | CO <sub>2</sub> : 0–100%<br>CH <sub>4</sub> : 0–50%<br>H <sub>2</sub> : 0–50%<br>CO: 0–100%                        | CO, CO <sub>2</sub> , CH <sub>4</sub> : 0,5%<br>from range or ± 3%<br>H <sub>2</sub> : ±5 ppm or 5% | 45 s to 90% step range            | [35]      |
| Wuhan Tianyu Intelligent Control Technology Co., Ltd. (TIANYU) | Syngas Analyzer Portable SYN-600                 | CO, CO <sub>2</sub> , CH <sub>4</sub> (NDIR)<br>H <sub>2</sub> (TCD - MEMS) | CO <sub>2</sub> : 0–100%<br>CH <sub>4</sub> : 0–100%<br>H <sub>2</sub> : 0–100%<br>CO: 0–10/100%                   | CO, CO <sub>2</sub> , CH <sub>4</sub> : ±2% FS<br>H <sub>2</sub> : ±3% FS                           | 45 s to 90% step range            | [36]      |
| MRU GmbH   | SWG 100 Syngas                                   | CO, CO <sub>2</sub> , CH <sub>4</sub> (NDIR)<br>H <sub>2</sub> (TCD)        | CO <sub>2</sub> : 0–10/100%<br>CH <sub>4</sub> : 0–10/100%<br>H <sub>2</sub> : 0–10/100%                           | no data   | no data                           | [37]      |
| ETG Risorse e Tecnologia S.r.l.                                | MCA 100 SYN P – Portable Syngas Analyzer         | CO, CO <sub>2</sub> , CH <sub>4</sub> (NDIR)<br>H <sub>2</sub> (TCD)        | Modified according to the needs of customer  | CO, CO <sub>2</sub> , CH <sub>4</sub> , H <sub>2</sub> : ±2% FS                                     | no data                           | [38]      |



## 5. Conclusions

The article presents a new method of monitoring the dry methane reforming process with the use of a matrix of chemical sensors. The matrix consisted of nine commercially available sensors (7 metal oxide sensors and 2 electrochemical) produced by Figaro Engineering Inc. Principal Component Regression (PCR) was used as a calibration method. The tests were performed on 117 model gas mixtures, characterized by the following process parameters: Inlet Molar Ratio (IMR) in the range 0.6–1.5, Outlet Molar Ratio (OMR) in the range 0.6–1.0, and Methane Conversion Level (MCL) in the range 80–95%. The best results (compared to gas chromatography) were obtained for OMR and MCL parameters—they did not exceed 1% of the parameter value. In the case of the IMR parameter, this error was about 7%.

We conclude that sensor matrices can be used on an industrial scale to supervise and control the ongoing process in real-time in order to automate process analytics. The use of sensor and sensor arrays for process control is becoming more and more popular and has a very high application potential, i.e., monitoring of biofiltration processes [28], bioreactors [39–41], quality assurance in the pharmaceutical industry [42], food industry [43,44] and odour monitoring [45]. It allows for a significant reduction in the cost of process control while maintaining the assumed accuracy of the obtained results.

**Author Contributions:** Conceptualization, B.S.; methodology, B.S.; software, B.S.; validation, B.S.; formal analysis, B.S. and J.G.; investigation, D.D., B.S. and T.D.; resources, B.S.; data curation, B.S.; writing—original draft preparation, D.D. and B.S.; writing—review and editing, B.S., T.D. and J.G.; visualization, D.D. and B.S.; supervision, B.S. and J.G.; funding acquisition, T.D. All authors have read and agreed to the published version of the manuscript.

**Funding:** This research was funded by the Ministry of Science and Higher Education, Poland, through the specific subsidy awarded to the Faculty of Chemistry, Gdańsk University of Technology, grant number 033878.

**Conflicts of Interest:** The authors declare no conflict of interest.

## References

1. Szulczyński, B.; Wasilewski, T.; Wojnowski, W.; Majchrzak, T.; Dymerski, T.; Namieśnik, J.; Gębicki, J. Different Ways to Apply a Measurement Instrument of E-Nose Type to Evaluate Ambient Air Quality with Respect to Odour Nuisance in a Vicinity of Municipal Processing Plants. *Sensors* **2017**, *17*, 2671. [[CrossRef](#)] [[PubMed](#)]
2. Gębicki, J.; Byliński, H.; Namieśnik, J. Measurement techniques for assessing the olfactory impact of municipal sewage treatment plants. *Environ. Monit. Assess.* **2016**, *188*, 1–17. [[CrossRef](#)] [[PubMed](#)]
3. Franchi, D.; Gonzatti, F.; Miotto, M.; Kuhn, V.; Farret, F. Use of infrared matrix sensor for temperature measurement and monitoring of PEM/FC stacks. *Sens. Actuators Phys.* **2019**, *293*, 119–127. [[CrossRef](#)]
4. Aguilera, T.; Lozano, J.; Paredes, J.A.; Álvarez, F.J.; Suárez, J.I. Electronic Nose Based on Independent Component Analysis Combined with Partial Least Squares and Artificial Neural Networks for Wine Prediction. *Sensors* **2012**, *12*, 8055–8072. [[CrossRef](#)]
5. Bachinger, T.; Mandenius, C.F. Searching for process information in the aroma of cell cultures. *Trends Biotechnol.* **2000**, *18*, 494–500. [[CrossRef](#)]
6. Bachinger, T.; Mandenius, C.F. Physiologically Motivated Monitoring of Fermentation Processes by Means of an Electronic Nose. *Eng. Life Sci.* **2001**, *1*, 33–42. [[CrossRef](#)]
7. Ghosh, S.; Tudu, B.; Bhattacharyya, N.; Bandyopadhyay, R. A recurrent Elman network in conjunction with an electronic nose for fast prediction of optimum fermentation time of black tea. *Neural Comput. Appl.* **2019**, *31*, 1165–1171. [[CrossRef](#)]
8. Hidayat, S.N.; Nuringtyas, T.R.; Triyana, K. Electronic Nose Coupled with Chemometrics for Monitoring of Tempeh Fermentation Process. In Proceedings of the 2018 4th International Conference on Science and Technology (ICST), Yogyakarta, Indonesia, 7–8 August 2018; pp. 1–6.
9. Kiani, S.; Minaei, S.; Ghasemi-Varnamkhasti, M. A portable electronic nose as an expert system for aroma-based classification of saffron. *Chemom. Intell. Lab. Syst.* **2016**, *156*, 148–156. [[CrossRef](#)]
10. Lidén, H.; Mandenius, C.F.; Gorton, L.; Meinander, N.Q.; Lundström, I.; Winquist, F. On-line monitoring of a cultivation using an electronic nose. *Anal. Chim. Acta* **1998**, *361*, 223–231. [[CrossRef](#)]
11. Li, G.; Yuan, L.; Wang, X.; Meng, Y.; Li, J.; Zhao, Y.; Peng, Y. Rapid quantification analysis of alcohol during the green jujube wine fermentation by electronic nose. In *IOP Conference Series: Earth and Environmental Science*; IOP Publishing: Bristol, UK, 2019; Volume 330, p. 052046.

12. Mandenius, C.F.; Eklöv, T.; Lundström, I. Sensor fusion with on-line gas emission multisensor arrays and standard process measuring devices in baker's yeast manufacturing process. *Biotechnol. Bioeng.* **1997**, *55*, 427–438. [CrossRef]
13. Tan, J.; Balasubramanian, B.; Sukha, D.; Ramkissoon, S.; Umaharan, P. Sensing fermentation degree of cocoa (*Theobroma cacao* L.) beans by machine learning classification models based electronic nose system. *J. Food Process. Eng.* **2019**, *42*, e13175. [CrossRef]
14. Tan, C.; Xie, D.; Liu, Y.; Peng, W.; Li, X.; Ai, L.; Wu, C.; Wen, C.; Huang, X.; Guo, J. Identification of different bile species and fermentation times of bile arisaema based on an intelligent electronic nose and least squares support vector machine. *Anal. Chem.* **2018**, *90*, 3460–3466. [CrossRef]
15. Belikova, V.; Panchuk, V.; Legin, E.; Melenteva, A.; Kirsanov, D.; Legin, A. Continuous monitoring of water quality at aeration plant with potentiometric sensor array. *Sens. Actuators Chem.* **2019**, *282*, 854–860. [CrossRef]
16. Oikonomou, P.; Botsialas, A.; Olziersky, A.; Stratakos, I.; Katsikas, S.; Dimas, D.; Sotiropoulos, G.; Goustouridis, D.; Raptis, I.; Sanopoulou, M. Wireless sensor network based on a chemocapacitive sensor array for the real-time monitoring of industrial pollutants. *Procedia Eng.* **2014**, *87*, 564–567. [CrossRef]
17. Giungato, P.; Di Gilio, A.; Palmisani, J.; Marzocca, A.; Mazzone, A.; Brattoli, M.; Giua, R.; De Gennaro, G. Synergistic approaches for odor active compounds monitoring and identification: State of the art, integration, limits and potentialities of analytical and sensorial techniques. *TRAC Trends Anal. Chem.* **2018**, *107*, 116–129. [CrossRef]
18. Gostelow, P.; Parsons, S. Sewage treatment works odour measurement. *Water Sci. Technol.* **2000**, *41*, 33–40. [CrossRef]
19. Gebicki, J.; Dymerski, T.; Rutkowski, S. Identification of odor of volatile organic compounds using classical sensory analysis and electronic nose technique. *Environ. Prot. Eng.* **2014**, *40*, 103–116. [CrossRef]
20. Di Francesco, F.; Lazzarini, B.; Marcelloni, F.; Pioggia, G. An electronic nose for odour annoyance assessment. *Atmos. Environ.* **2001**, *35*, 1225–1234. [CrossRef]
21. IV, E.A.B.; Koziel, J.A.; Cai, L.; Wright, D. Characterization of Livestock Odors Using Steel Plates, Solid-Phase Microextraction, and Multidimensional Gas Chromatography–Mass Spectrometry–Olfactometry. *J. Air Waste Manag. Assoc.* **2006**, *56*, 1391–1403. [CrossRef]
22. Zarra, T.; Naddeo, V.; Belgiorno, V.; Reiser, M.; Kranert, M. Instrumental characterization of odour: a combination of olfactory and analytical methods. *Water Sci. Technol.* **2009**, *59*, 1603–1609. [CrossRef]
23. Dincer, F.; Odabasi, M.; Muezzinoglu, A. Chemical characterization of odorous gases at a landfill site by gas chromatography–mass spectrometry. *J. Chromatogr.* **2006**, *1122*, 222–229. [CrossRef] [PubMed]
24. Ferrari, G.; Lablanquie, O.; Cantagrel, R.; Ledauphin, J.; Payot, T.; Fournier, N.; Guichard, E. Determination of key odorant compounds in freshly distilled cognac using GC-O, GC-MS, and sensory evaluation. *J. Agric. Food Chem.* **2004**, *52*, 5670–5676. [CrossRef] [PubMed]
25. Munoz, R.; Sivret, E.C.; Parcsi, G.; Lebrero, R.; Wang, X.; Suffet, I.M.; Stuetz, R.M. Monitoring techniques for odour abatement assessment. *Water Res.* **2010**, *44*, 5129–5149. [CrossRef] [PubMed]
26. Patel, H.K. *The Electronic Nose: Artificial Olfaction Technology*; Springer: New Delhi, India, 2014.
27. Principal Components Regression. Available online: <http://www.science.smith.edu/~jcrouser/SDS293/labs/lab11-r.html> (accessed on 30 June 2021).
28. Szulczyński, B.; Rybarczyk, P.; Gebicki, J. Monitoring of n-butanol vapors biofiltration process using an electronic nose combined with calibration models. *Monatshefte Chem. Chem. Mon.* **2018**, *149*, 1693–1699. [CrossRef] [PubMed]
29. Tan, J.; Xu, J. Applications of electronic nose (e-nose) and electronic tongue (e-tongue) in food quality-related properties determination: A review. *Artif. Intell. Agric.* **2020**, *4*, 104–115. [CrossRef]
30. Abdulrazzaq, N.N.; Al-Sabbagh, B.H.; Rees, J.M.; Zimmerman, W.B. Measuring Vapor and Liquid Concentrations for Binary and Ternary Systems in a Microbubble Distillation Unit via Gas Sensors. *Chemosensors* **2018**, *6*, 31. [CrossRef]
31. Portable Infrared Syngas Analyzer Gasboard-3100P. Available online: [https://en.gassensor.com.cn/GasAnalyzer/info\\_itemid\\_25\\_2.html](https://en.gassensor.com.cn/GasAnalyzer/info_itemid_25_2.html) (accessed on 30 June 2021).
32. Syngas Analysis System Gasboard-9021. Available online: [https://en.gassensor.com.cn/GasAnalyzer/info\\_itemid\\_283.html](https://en.gassensor.com.cn/GasAnalyzer/info_itemid_283.html) (accessed on 30 June 2021).
33. Portable Natural Gas Analyzer Gasboard-3110P. Available online: <http://www.gas-analyzers.com/products/syngas-analyzer/Gasboard-3110P.html> (accessed on 30 June 2021).
34. 970P Portable Multi-Gas Industrial Analyzers. Available online: <https://catalog.nova-gas.com/viewitems/ication-specific-product-lines-syngas-gasification/strial-syngas-analyzers-and-gasification-analyzers> (accessed on 30 June 2021).
35. Online Syngas Analyzer by Vasthi. Available online: <https://www.vasthi.com/online-syngas-analyzer> (accessed on 30 June 2021).
36. Syngas Analyzer Portable SYN-600. Available online: <https://www.syngas-analyzer.com/product/Syngas-Analyzer-Portable-SYN-600.html> (accessed on 30 June 2021).
37. SWG 100 Syngas. Available online: <https://www.mru.eu/en/products/detail/swg-100-syngas-1/> (accessed on 30 June 2021).
38. MCA 100 SYN P—Portable Syngas Analyzer. Available online: <https://www.energy-xprt.com/products/etg-model-mca-100-syn-p-portable-syngas-analyzer-525843> (accessed on 30 June 2021).
39. Gruber, P.; Marques, M.P.C.; Szita, N.; Mayr, T. Integration and application of optical chemical sensors in microbioreactors. *Lab Chip* **2017**, *17*, 2693–2712. [CrossRef] [PubMed]
40. Demuth, C.; Varonier, J.; Jossen, V.; Eibl, R.; Eibl, D. Novel probes for pH and dissolved oxygen measurements in cultivations from millilitre to benchtop scale. *Appl. Microbiol. Biotechnol.* **2016**, *100*, 3853–3863. [CrossRef]



41. Wang, X.d.; Wolfbeis, O.S. Optical methods for sensing and imaging oxygen: materials, spectroscopies and applications. *Chem. Soc. Rev.* **2014**, *43*, 3666–3761. [[CrossRef](#)]
42. Spichiger, S.; Spichiger-Keller, U.E. Process Monitoring with Disposable Chemical Sensors Fit in the Framework of Process Analysis Technology (PAT) for Innovative Pharmaceutical Development and Quality Assurance. *Chim. Int. J. Chem.* **2010**, *64*, 803–807. [[CrossRef](#)]
43. Pearce, T.C.; Gardner, J.W.; Friel, S.; Bartlett, P.N.; Blair, N. Electronic nose for monitoring the flavour of beers. *Analyst* **1993**, *118*, 371–377. [[CrossRef](#)]
44. Gardner, J.W.; Shin, H.W.; Hines, E.L.; Dow, C.S. An electronic nose system for monitoring the quality of potable water. *Sensors Actuators Chem.* **2000**, *69*, 336–341. [[CrossRef](#)]
45. Romero-Flores, A.; McConnell, L.L.; Hapeman, C.J.; Ramirez, M.; Torrents, A. Evaluation of an electronic nose for odorant and process monitoring of alkaline-stabilized biosolids production. *Chemosphere* **2017**, *186*, 151–159. [[CrossRef](#)] [[PubMed](#)]

