

Experimental study on the effect of selected sterilization methods on mechanical properties of polylactide FFF specimens

Journal:	<i>Rapid Prototyping Journal</i>
Manuscript ID	RPJ-05-2021-0115.R3
Manuscript Type:	Original Article
Keywords:	Mechanical properties, Sterilization, Polylactide, Fused filament fabrication, UV light sterilization, Ethylene oxide sterilization

SCHOLARONE™
Manuscripts

Author accepted manuscript of:

Andrzejewska, A.J. (2022), "Experimental study on the effect of selected sterilization methods on mechanical properties of polylactide FFF specimens", Rapid Prototyping Journal, Vol. ahead-of-print No. ahead-of-print. <https://doi.org/10.1108/RPJ-05-2021-0115>

This author accepted manuscript is deposited under a Creative Commons Attribution Non-commercial 4.0 International (CC BY-NC) licence. This means that anyone may distribute, adapt, and build upon the work for non-commercial purposes, subject to full attribution. If you wish to use this manuscript for commercial purposes, please contact permissions@emerald.com

Experimental study on the effect of selected sterilization methods on mechanical properties of polylactide FFF specimens

Abstract

Purpose: Biodegradable polymers are widely used in personalized medical devices or scaffolds for tissue engineering. The manufacturing process should be finished with sterilization procedure. However, it is not clear how the different sterilization methods have an impact on the mechanical strength of the 3D printed parts, like bone models or personalized mechanical devices. This manuscript presents the results of mechanical testing of polylactide based bone models before and after sterilization.

Design/methodology/approach: Polylactide specimens prepared in fused filament fabrication technology were sterilized with different sterilization methods: ultraviolet and ethylene oxide. Mechanical properties were determined by testing tensile strength, Young modulus and toughness.

Findings: The tensile strength of material after sterilization was significantly higher after ethylene oxide sterilization compared to the ultraviolet sterilization, but in both sterilization methods the specimens characterized lower tensile strength and Young modulus when compared to the control. In comparison of toughness results there was no statistically significant differences. The findings are particularly significant in the perspective of using individual implants, bone grafts and dental guides.

Originality: Although FFF 3D printing devices equipped with UV light sterilization options are available, experimental results of the effect of selected sterilization methods on the mechanical strength of additively manufactured parts have not been described. This paper completes the present state of the art on the problem of sterilization of FFF parts from biodegradable materials.

Keywords Mechanical properties, Sterilization, Polylactide, Fused filament fabrication, UV light sterilization, Ethylene oxide sterilization

Paper type Research paper

List of abbreviations

- 3D – three-dimensional
- CO₂ laser – carbon dioxide laser
- EtO – ethylene oxide
- H₂O₂ – hydrogen peroxide
- HDPE – high density polyethylene
- kGy – Gray (unit)
- MHAp – mackerel fish hydroxyapatite
- PA – Peracetic Acid
- PCL – polycaprolactone
- PLA – polylactic acid
- PLCL – poly-L-lactide-co-ε-caprolactone
- PLGA – poly(lactide co-glycolide)
- TMPTMA – trimethylpropane trimethacrylate
- TPU – thermoplastic polyurethane
- UV – ultraviolet

1. Introduction

The expansion of the three-dimensional printing technology has resulted in a wide range of applications, e.g. in biomedical applications, for implantology (Singh *et al.*, 2019; Vasamsetty *et al.*, 2020), bone defect replacements (Andrzejewska, 2019; Bose *et al.*, 2013; Ghorbani *et*

1
2
3 1 *al.*, 2020) or personalized mechanical devices (Sapoval *et al.*, 2020; Wesemann *et al.*, 2020).
4 2 The safety of implantable materials should respect a number of standards related to **the**
5 3 biocompatibility, proper mechanical properties but in addition, the microbiological safety aspect
6 4 seems to be the most important. For this reason, ready-to-use products including personalized
7 5 medical devices and implantable materials are sterilized.

8 6 The mechanical properties of 3D printed bone models or other personalized medical devices
9 7 are crucial for its application. The above-mentioned properties may be affected by properties
10 8 on each stage of manufacturing process like storage of materials, environmental factors during
11 9 processing, postprocessing sterilization. Also different methods of sterilization of polymer
12 10 materials applied in biomedical solutions are used. The different sterilization methods can
13 11 affect changes in mechanical properties.

14 12 Tipnis and Burgess (2018) recognized and developed methods of sterilization of polymeric
15 13 materials for biomedical applications. Following methods include: ethylene oxide, radiation, dry
16 14 and heat steam, H₂O₂ and ozone, also peracetic acid, UV light, microwave, sound waves and
17 15 pulsed light.

18 16 The study conducted by Haim Zada *et al.* (2019) describes the effect of ethylene oxide
19 17 sterilization and gamma sterilization on the behavior of Poly-L-lactide-co-ε-caprolactone
20 18 (PLCL) specimens prepared in the multicycle dip-coating process. The main conclusion of the
21 19 researchers is the recommendation of EtO sterilization instead of gamma-radiation for PLCL
22 20 balloon implants. Chen *et al.* (2019) described the stability of specimens made of high density
23 21 polyethylene (HDPE) and Polyamide 6 and exposed to two sterilization methods - novel
24 22 vaporized hydrogen peroxide and electron beam processes. The specimens were prepared
25 23 both by additive manufacturing and by injection molding. The research presented by the
26 24 authors proved that injection molded specimens were more stable than 3D printed specimens
27 25 upon sterilization processes.

28 26 Ng *et al.* (2019) reported the effect of electron beam irradiation at room temperature on the
29 27 properties of compression-formed PLA in combination with fish bone waste mackerel (MHAp)
30 28 and trimethylpropane trimethacrylate (TMPTMA). The authors noted that when the radiation
31 29 dose increased, the mechanical properties of the composite improved due to better
32 30 crosslinking. Meanwhile, in the case of pure PLA, increasing the radiation dose contributed to
33 31 a decrease in strength.

34 32 Artemenko *et al.* (2012) investigated the influence of sterilization methods such as dry heat,
35 33 autoclave and UV radiation on chemical and biological properties of plasma polymers. General
36 34 finding of the work was conclusion that there exists no universal sterilization method that
37 35 assures preservation of the properties of all kinds of plasma polymers.

38 36 Davison *et al.* (2018) discussed the results of tests performed on specimens of poly(lactide co-
39 37 glycolide) PLGA prepared by compression molding. Specimens were gamma sterilized at
40 38 40 kGy and room temperature or low temperature (-80°C) in a nitrogen atmosphere. The
41 39 results reported that the molecular weight was significantly reduced, as was the glass transition
42 40 temperature, which indicates a chain rupture. FTIR reported minor changes in the chemical
43 41 structure in methyl and carbonyl groups after irradiation. The glass transition temperature
44 42 changed significantly between irradiation at -80°C and irradiation at 25°C, but this difference
45 43 was only 1°C. Consequently, the results indicate that the applied sterilization temperature does
46 44 not affect PLGA when carried out in a nitrogen atmosphere.

47 45 Polymeric Tissue Engineering Scaffolds in Yoganarasimha *et al.* (2019) research were
48 46 prepared by electrospinning method from polycaprolactone (PCL) was sterilized with Peracetic
49 47 Acid (PA). The main goal of the study was to determine the effect of the selected sterilization
50 48 method on the cytotoxicity of PCL scaffolds. It has been shown that the rinsing of scaffolds in
51 49 80% ethanol for 30 minutes effectively eliminates toxic PA waste and restores **the**
52 50 cytocompatibility.

1
2
3 1 De Cassan et al. (2019) work presents scaffolds manufactured from PCL were also produced
4 2 by electrospinning and then sterilized using three methods, i.e. electron beam, gamma
5 3 radiation and Röntgen radiation. It was shown that the dose of radiation had a significant effect
6 4 on changes in molecular mass and degree of crystallinity, whereas the type of used radiation
7 5 had no significant effect on changes in mechanical behaviour.

8 6 Preem et al. (2019) reported study of scaffolds manufactured with the PCL electrospinning
9 7 method. The generated scaffolds were exposed to UV-sterilization, gamma-irradiation,
10 8 chlorine gas. It was observed that gamma sterilization increased the hardness and elasticity
11 9 of PCL constructs as a result of increased crystallinity of the polymer.

12 10 Rainer et al. (2010) used in research constructions performed with the method of
13 11 electrospinning from polylactide, which were exposed to soaking in absolute ethanol, dry oven
14 12 and autoclave treatments, UV irradiation, and hydrogen peroxide gas plasma treatment. The
15 13 study disclosed that UV irradiation and hydrogen peroxide gas plasma are the most effective
16 14 sterilization techniques, which ensure sterility of the electrospun scaffolds without affecting **the**
17 15 chemical and morphological features.

18 16 In view of the work described below, it can be stated that various sterilization methods can be
19 17 successfully used to sterilize the thermoplastic polymers. Nevertheless, the field of effect of
20 18 sterilization methods on structural components made by additive manufacturing methods is
21 19 still not well understood. There are single literature reports demonstrating the proper way of
22 20 sterilization of porous constructions produced by additive manufacturing methods. Luchini et
23 21 al. (2021) describes results of sterilization with heat-based methods and sanitizing with
24 22 various chemical solutions of 3D printed polylactic acid (PLA) or thermoplastic polyurethane
25 23 (TPU) parts. This study shows that while personal protective equipment is produced using PLA
26 24 and the traditional infill-based patterns model may be initially sterile, re-sterilization is not
27 25 possible using methods such as isopropanol, bleach, and/or H₂O₂. In addition, autoclaving is
28 26 technique typically utilized to sanitize a variety of materials, but it isn't suitable for PLA and
29 27 TPU 3D printed parts.

30 28 In the manuscript Pérez Davila et al. (2021) the analyzed how the most common techniques
31 29 used to sterilize PLA medical devices are affecting the physicochemical and biocompatible
32 30 properties of 3D printed items.

33 31 It has been observed that EtO sterilization is the most universal and the most widespread
34 32 method of low-temperature sterilization in large clinical centers (Boiano and Steege, 2015;
35 33 Sobaszek et al., 1999). Also it is considered to be the method with high effectiveness, low cost.
36 34 While UV methods are used in small rural clinics (Rutala and Weber, 2015), dental practices
37 35 (Cumbo et al., 2020) or beauty salons (Sowah and Ahiabor, 2014). Moreover, manufacturers
38 36 of 3D printers offer devices equipped with the possibility of UV sterilization during printing.
39 37 Therefore, the objective of this study was to investigate the effect of sterilization methods: UV
40 38 light and ethylene oxide on the mechanical properties of 3D printed components produced
41 39 from biodegradable polylactide. The results of testing the mechanical properties of sterilized
42 40 parts are important for research and development in regenerative medicine and medical
43 41 devices, which must be biologically safe for users. The preliminary study of mechanical
44 42 properties that was conducted should result in the most suitable method for sterilization of 3D
45 43 printed parts, to be used in future studies on the effectivity of sterilization methods.

46 44 47 45 **2. Methodology**

48 46 Dog-bone shaped specimens were used to determine changes in the mechanical behavior of
49 47 3D printed polymeric materials and then sterilized. The geometry and optimal parameters of
50 48 fused filament fabrication are similar as in further research (Andrzejewska, 2021;
51 49 Andrzejewska et al., 2019). For this experiment, commercially available 3DXPLA007-EA
52 50 polylactide (Sigma-Aldrich, Saint Louis, MO, USA) was applied. Specimens were prepared
53 51 with the method of fused filament fabrication, on a 3D printer Kreator Motion (Krakow, Poland).

Printing of elements was based on the planned density of cross-sectional infill equal to 100% and the angular placement of material fibres in relation to the specimen axis, i.e. $+45^\circ/-45^\circ$. The specimen shape and geometry based on (ISO 527-2:2012, 2012) standard is presented in Figure 1. However, the 3D printing settings of dog-bone shaped specimen are summarized in Table 1.

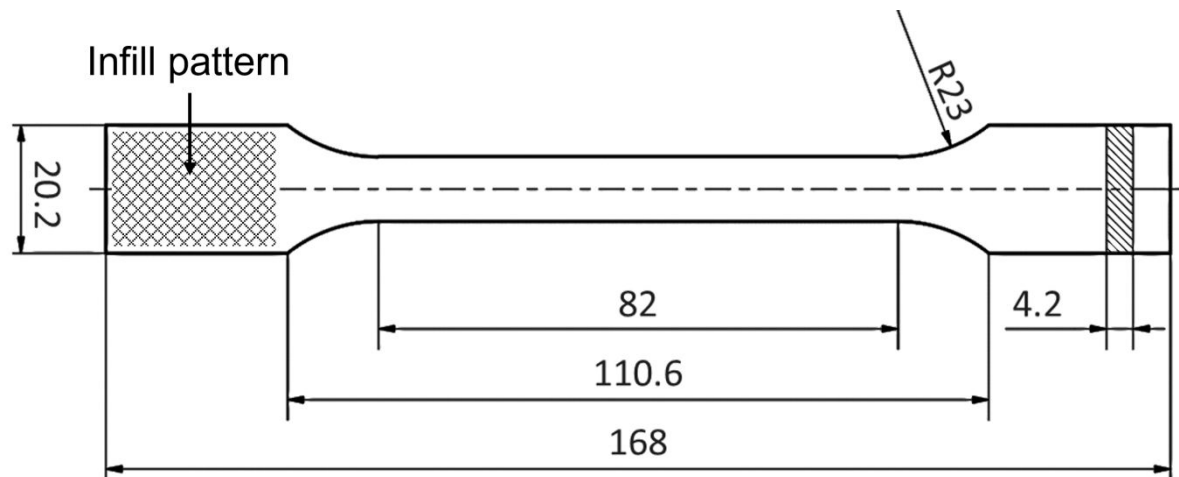


Figure 1. Geometry of dog-bone shaped specimen.

Table 1. 3D printing parameters

No.	Selected parameters	Value
1.	Nozzle temperature	200°C
2.	Bed temperature	65°C
3.	Nozzle diameter	0.4 mm
4.	Filament diameter	1.75 mm
5.	Layer thickness	0.1 mm
6.	Fiber orientation to specimen axis	$+45^\circ/-45^\circ$
7.	Outline	2
8.	Top/bottom solid layers	6/6

Two methods of sterilization were chosen, i.e. UV light sterilization and ethylene oxide sterilization. The process of sterilization based on "Guideline for Disinfection and Sterilization in Healthcare Facilities" of Centres for Disease Control and Prevention. Sterilization with ultraviolet radiation was conducted in UV-C sterilizer (Activ, Wroclaw, Poland), using UV radiation of 254 nm wavelength. The time of sterilization of the specimens was 30 minutes and the process was established at 60°C. The UV sterilized forms were deposited in a desiccator filled with silica gel for 24 hours. However, the second group of specimens were sterilized with ethylene oxide in Steri-Vac Sterilizer (3M, Saint Paul, MN, USA). The following process parameters were defined: gas concentration - 450 mg/l; temperature - 55°C; relative humidity - 60%; exposure time - 60 min. Subsequently, after exposure to the sterilizing agent, the specimens were subjected to a degasification period lasting 12 hours in the sterilizer chamber. The tests of mechanical properties were performed on the INSTRON ElectroPuls E3000 (Norwood, MA, USA) tensile machine with an electromagnetic actuator of ± 3 kN force. The traverse speed of the testing machine was 1 mm/min. Tests of material's mechanical properties to uniaxial tensile strength before and after sterilization with two methods were realized at room

1
2
3 1 temperature. In each group of tests, 5 specimens were subjected to mechanical properties
4 2 measurements (Andrzejewska *et al.*, 2019; ISO 527-2:2012, 2012)
5 3

4 3. Results and discussion

5 Three parameters were used in the analysis of the influence of the selected sterilization method
6 on changes in mechanical behavior of the biodegradable material. The tensile mechanical
7 behavior of the sterilized polylactide parts was determined: ultimate tensile strength (σ_m),
8 Young's modulus (E) and toughness i.e. the amount of absorbed energy needed to break the
9 specimen (Q) (Jyoti *et al.*, 2022; Mohammadi *et al.*, 2017; Yang *et al.*, 2019). The toughness
10 is parameter expressed by the Equation (1).

$$Q = \int_t \sigma d\varepsilon \quad (1)$$

11
12 Figure 2 presented representative cases of stress-strain curves of non-sterilized control
13 specimens and specimens exposed to two different methods of sterilization. On the grounds
14 of the presented charts it can be observed that specimens before sterilization were
15 characterized by the greatest value of tensile strength and the greatest elongation. However,
16 the specimens after sterilization, in relation to the selected method, were characterized by
17 reduced strength and elongation in comparison with non-sterilized specimens. Higher values
18 of strength and elongation were reported for specimens after ethylene oxide sterilization.
19 Temperature-induced sterilization contributes to scission of the polymer chain, which results
20 in reduced tensile strength and elongation (Otaguro *et al.*, 2010; Papadimitriou *et al.*, 2021).
21 In the process of determining the statistical significance of differences, the recorded and
22 calculated values of mechanical parameters were collected and then the results were
23 analyzed. Table 2 summarizes the mean value, standard deviation and median of the
24 determined strength parameters. The coefficient of variation of results received for the three
25 selected parameters was determined for each group of tested specimens. Besides, the
26 statistical significance of differences in results between individual groups of specimens was
27 compared. Estimates of statistical significance of the differences were performed using
28 GraphPad Prism. Comparison of specimens before and after sterilization by two methods was
29 performed by one-way ANOVA test and post-hoc Fisher's LSD test. The analysis was carried
30 out at the significance level of $p < 0.05$ (Norani *et al.*, 2021; Zhu *et al.*, 2021).
31

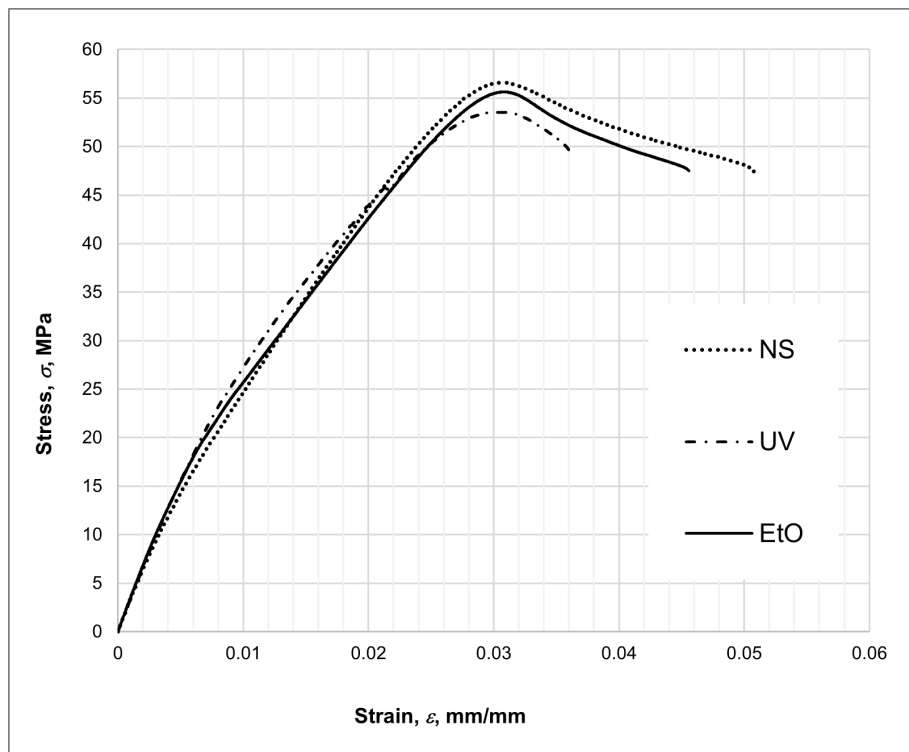


Figure 2. The representative stress–strain curves of the specimens before (NS) and after UV light or EtO sterilization.

Table 2. Calculated values of tensile strength parameters

PLA part	Ultimate Tensile Strength, σ_M , MPa		Young modulus, E , MPa		Toughness, Q , MJ/m ³	
	Mean \pm STD	Median	Mean \pm STD	Median	Mean \pm STD	Median
Non-sterilised	57.92 \pm 0.66	58.22	3585.45 \pm 123.32	3598.36	1.007 \pm 0.004	1.021
UV light-sterilised	53.38 \pm 0.16	53.37	3116.28 \pm 195.01	3045.35	1.080 \pm 0.060	1.049
EtO-sterilised	55.54 \pm 0.47	55.55	3121.81 \pm 216.14	3121.92	1.059 \pm 0.090	1.040

In case of the analysis of the coefficient of variation of results in each group of specimens, the coefficient value was lower than 10% regardless of the analyzed parameter. Statistical comparison of differences in specific parameters between groups of non-sterilized and UV or ethylene oxide sterilized specimens showed statistically significant differences in tensile strength (p -value < 0.0001). Furthermore, statistically significant differences in Young modulus were shown in comparison of specimens before and after sterilization by both methods (p -value = 0.0017). However, there were no statistically significant differences in changes in Young modulus between the specimens that were sterilized (p -value = 0.9626). When comparing toughness results, no statistically significant differences were found between samples before and after sterilization with both methods.

Figure 3 shows a comparison of several groups of specimens in relation to parameters reached in a tensile test and calculated on the basis of experimental data.

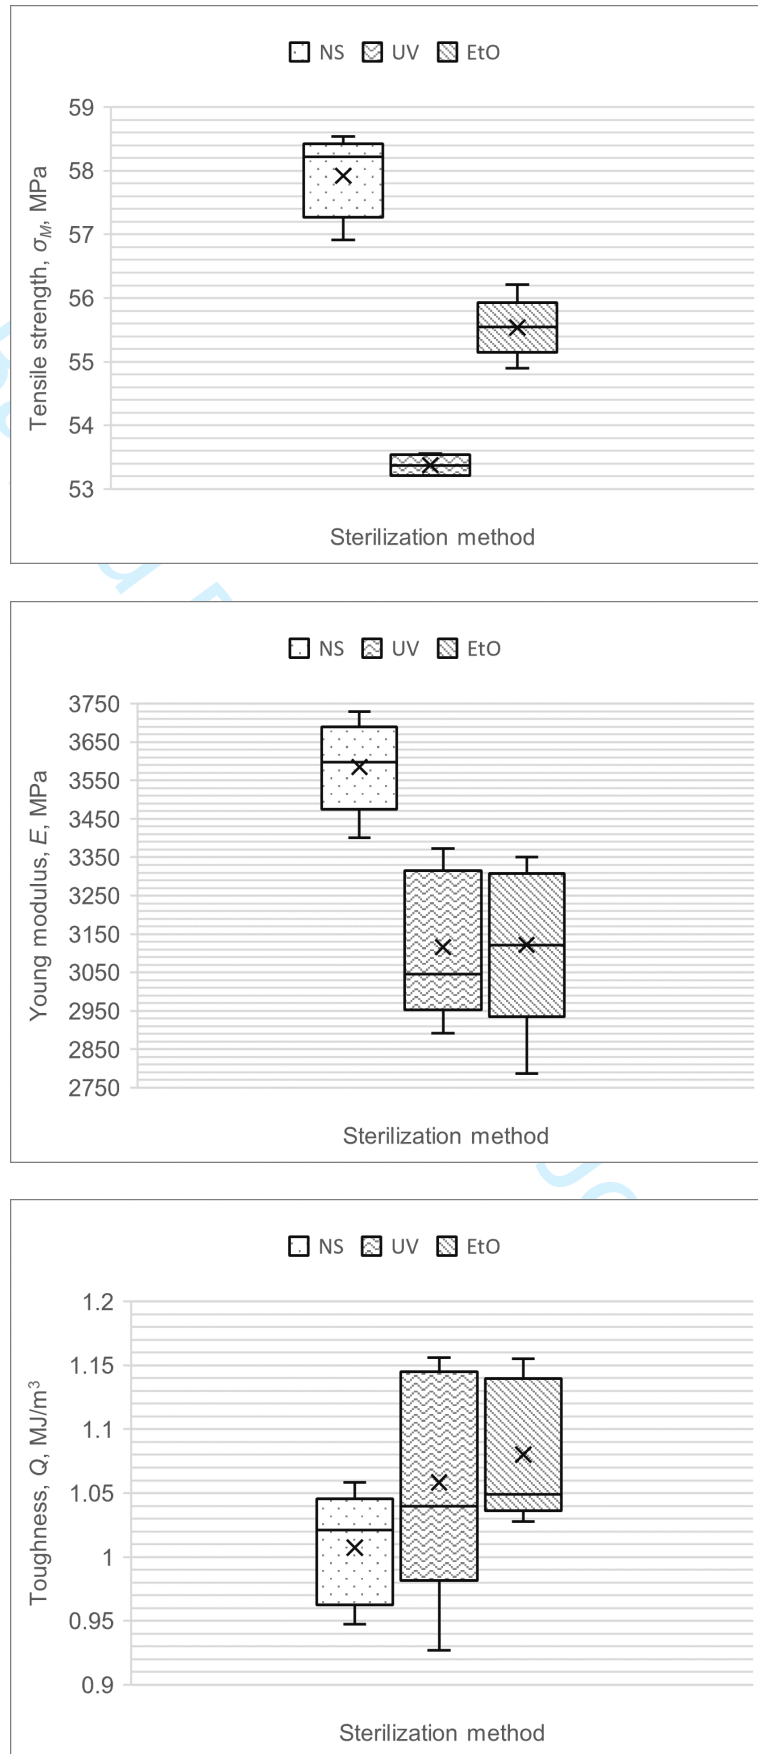


Figure 3. Comparison of mechanical properties: a) tensile strength, b) Young modulus, c) toughness.

Although statistically significant differences in tensile strength values have been shown between non-sterilized and sterilized specimens with different methods, the reduction in strength values does not exceed 2 MPa for EtO sterilization and respectively 4 MPa for UV sterilization. The results obtained after EtO sterilization are very similar to the results obtained by other researchers in publication (Zhao *et al.*, 2019), whereas the expected strength value of the material may be varied and may depend on the method of specimens preparation, grade of material, content of two forms of the monomeric acid (D-or L-lactic acid) etc. The stress and strain values in printed specimens will be affected by the printing temperature and then the sterilization temperature. The effect of heating strongly influences the changes of polymeric bonds in the entire specimen. As noted Grasso *et al.* (2018) stress redistribution is crucial in tests on specimens previously treated with temperatures close to the glass transition temperature of PLA and then cooled.

The important parameter found in tests presented in this research is toughness, which determines the specimen's susceptibility to fracture. In the documents of other scientists, no information was found regarding the determination of toughness parameter, specifically its changes due to the sterilization of biodegradable 3D printed material.

5. Conclusions

The results of the research presented in this paper compared the influence of the method of sterilization on mechanical properties of biodegradable material.

- The obtained results provided, in general, a lower strength of the sterilized specimens.
- The reduction in strength value from 2 to 4 MPa should not be considered as a disincentive to sterilize 3D printed elements.
- The geometry of the specimens was measured before and after sterilization. Changes in geometrical dimensions (cross-sectional area) did not exceed 10%. Value of the cross-sectional area after sterilization was taken for strength calculations. Due to the effect of temperature (close to glass transition temperature), a change in the ordering of polymer chains and crystalline transformations may have occurred, but further studies are necessary to confirm above.

Based on mechanical properties both EtO and UV light sterilization are suitable for sterilizing bone models or personalized medical devices. EtO sterilization results in lower strength loss and is declared in literature as more microbiologically effective than UV. The effectiveness of sterilization 3D printed parts will be evaluated in future research.

Supplementary Materials: not applicable

Author Contributions: It is single-authored paper.

Funding: This research received no external funding.

Conflicts of Interest: The authors declare no conflicts of interest.

References

- Andrzejewska, A. (2019), "Biomechanical properties of 3D-printed bone models", *BioSystems*, available at:<https://doi.org/10.1016/j.biosystems.2019.01.001>.
- Andrzejewska, A. (2021), *Three-Dimensional Printing of Bone Models, Advances in Intelligent Systems and Computing*, Vol. 1223, available at:https://doi.org/10.1007/978-3-030-52180-6_1.
- Andrzejewska, A., Pejkowski, Ł. and Topoliński, T. (2019), "Tensile and Fatigue Behavior of Additive Manufactured Polylactide", *3D Printing and Additive Manufacturing*, Vol. 6 No. 5, pp. 272–280.
- Artemenko, A., Kylián, O., Choukourov, A., Gordeev, I., Petr, M., Vandrovcová, M., Polonskyi, O., *et al.* (2012), "Effect of sterilization procedures on properties of plasma

- 1
2
3 1 polymers relevant to biomedical applications”, *Thin Solid Films*, Vol. 520 No. 24, pp.
4 2 7115–7124.
- 5 3 Boiano, J.M. and Steege, A.L. (2015), “Ethylene Oxide and Hydrogen Peroxide Gas Plasma
6 4 Sterilization: Precautionary Practices in U.S. Hospitals.”, *Zentralsterilisation*
7 5 (*Wiesbaden*), Vol. 23 No. 4, pp. 262–268.
- 8 6 Bose, S., Vahabzadeh, S. and Bandyopadhyay, A. (2013), “Bone tissue engineering using
9 7 3D printing”, *Materials Today*, Elsevier Ltd., Vol. 16 No. 12, pp. 496–504.
- 10 8 de Cassan, D., Hoheisel, A.L., Glasmacher, B. and Menzel, H. (2019), “Impact of sterilization
11 9 by electron beam, gamma radiation and X-rays on electrospun poly-(ϵ -caprolactone)
12 10 fiber mats”, *Journal of Materials Science: Materials in Medicine*, Springer US, Vol. 30
13 11 No. 4, pp. 1–11.
- 14 12 Chen, Y., Neff, M., McEvoy, B., Cao, Z., Pezzoli, R., Murphy, A., Gately, N., *et al.* (2019), “3D
15 13 printed polymers are less stable than injection moulded counterparts when exposed to
16 14 terminal sterilization processes using novel vaporized hydrogen peroxide and electron
17 15 beam processes”, *Polymer*, Vol. 183, p. 121870.
- 18 16 Cumbo, E., Gallina, G., Messina, P. and Scardina, G.A. (2020), “Alternative methods of
19 17 sterilization in dental practices against COVID-19”, *International Journal of*
20 18 *Environmental Research and Public Health*, Vol. 17 No. 16, pp. 1–14.
- 21 19 Davison, L., Themistou, E., Buchanan, F. and Cunningham, E. (2018), “Low temperature
22 20 gamma sterilization of a bioresorbable polymer, PLGA”, *Radiation Physics and*
23 21 *Chemistry*, Elsevier Ltd, Vol. 143, pp. 27–32.
- 24 22 Ghorbani, F., Li, D., Ni, S., Zhou, Y. and Yu, B. (2020), “3D printing of acellular scaffolds for
25 23 bone defect regeneration: A review”, *Materials Today Communications*, Vol. 22, p.
26 24 100979.
- 27 25 Grasso, M., Azzouz, L., Ruiz-Hincapie, P., Zarrelli, M. and Ren, G. (2018), “Effect of
28 26 temperature on the mechanical properties of 3D-printed PLA tensile specimens”, *Rapid*
29 27 *Prototyping Journal*, Vol. 24 No. 8, pp. 1337–1346.
- 30 28 Haim Zada, M., Kumar, A., Elmalak, O., Mechrez, G. and Domb, A.J. (2019), “Effect of
31 29 Ethylene Oxide and Gamma (γ -) Sterilization on the Properties of a PLCL Polymer
32 30 Material in Balloon Implants”, *ACS Omega*, Vol. 4 No. 25, pp. 21319–21326.
- 33 31 “ISO 527-2:2012 Plastics — Determination of tensile properties — Part 2: Test conditions for
34 32 moulding and extrusion plastics”. (2012), .
- 35 33 Jyoti, A., Shaikeea, D., Cambridge, U.K. and Angeles, L. (2022), “Mechanical metamaterials :
36 34 Toughness and design criteria”, No. February, pp. 1–6.
- 37 35 Luchini, K., Sloan, S.N.B., Mauro, R., Sargsyan, A., Newman, A., Persaud, P., Hawkins, D.,
38 36 *et al.* (2021), “Sterilization and sanitizing of 3D-printed personal protective equipment
39 37 using polypropylene and a Single Wall design”, *3D Printing in Medicine*, 3D Printing in
40 38 Medicine, Vol. 7 No. 1, pp. 1–10.
- 41 39 Mohammadi, P., Toivonen, M.S., Ikkala, O., Wagermaier, W. and Linder, M.B. (2017),
42 40 “Aligning cellulose nanofibril dispersions for tougher fibers”, *Scientific Reports*, Springer
43 41 US, Vol. 7 No. 1, pp. 1–11.
- 44 42 Ng, H.M., Bee, S.T., Sin, L.T., Ratnam, C.T. and Rahmat, A.R. (2019), “Effect of electron
45 43 beam irradiation sterilization on biomedical polylactic acid composite filled with
46 44 *Scomberomorus Guttatus*-derived hydroxyapatite”, *Composites Part B: Engineering*,
47 45 Elsevier Ltd, Vol. 176 No. October 2018, p. 107273.
- 48 46 Norani, M.N.M., Abdollah, M.F. Bin, Abdullah, M.I.H.C., Amiruddin, H., Ramli, F.R. and
49 47 Tamaldin, N. (2021), “3D printing parameters of acrylonitrile butadiene styrene polymer
50 48 for friction and wear analysis using response surface methodology”, *Proceedings of the*
51 49 *Institution of Mechanical Engineers, Part J: Journal of Engineering Tribology*, Vol. 235
52 50 No. 2, pp. 468–477.
- 53 51 Otaguro, H., de Lima, L.F.C.P., Parra, D.F., Lugão, A.B., Chinelatto, M.A. and Canevarolo,
54 52 S. V. (2010), “High-energy radiation forming chain scission and branching in
55 53 polypropylene”, *Radiation Physics and Chemistry*, Vol. 79 No. 3, pp. 318–324.
- 56 54 Papadimitriou, C., Melidis, L., Kotoulas, L., Makris, N. and Katakalos, K. (2021),
57 55 “Thermomechanical Characterization of CFRPs under Elevated Temperatures for

- 1
2
3 1 Strengthening Existing Structures”, *Fibers*, Vol. 9 No. 12, available
4 2 at:<https://doi.org/10.3390/fib9120080>.
- 5 3 Pérez Davila, S., González Rodríguez, L., Chiussi, S., Serra, J. and González, P. (2021),
6 4 “How to sterilize polylactic acid based medical devices?”, *Polymers*, Vol. 13 No. 13, pp.
7 5 1–18.
- 8 6 Preem, L., Vaarmets, E., Meos, A., Jõgi, I., Putrinš, M., Tenson, T. and Kogermann, K.
9 7 (2019), “Effects and efficacy of different sterilization and disinfection methods on
10 8 electrospun drug delivery systems”, *International Journal of Pharmaceutics*, Vol. 567
11 9 No. April, available at:<https://doi.org/10.1016/j.ijpharm.2019.118450>.
- 12 10 Rainer, A., Centola, M., Spadaccio, C., Gherardi, G., Genovese, J.A., Licocchia, S. and
13 11 Trombetta, M. (2010), “Comparative study of different techniques for the sterilization of
14 12 poly-L-lactide electrospun microfibers: Effectiveness vs. material degradation”,
15 13 *International Journal of Artificial Organs*, Vol. 33 No. 2, pp. 76–85.
- 16 14 Rutala, W.A. and Weber, D.J. (2015), “Control of Hospital Waste”, *Mandell, Douglas, And*
17 15 *Bennett’S Principles And Practice Of Infectious Diseases*, No. January, pp. 3294–3309.
- 18 16 Sapoval, M., Gaultier, A.L., Del Giudice, C., Pellerin, O., Kassis-Chikhani, N., Lemarteleur,
19 17 V., Fouquet, V., *et al.* (2020), “3D-printed face protective shield in interventional
20 18 radiology: Evaluation of an immediate solution in the era of COVID-19 pandemic”,
21 19 *Diagnostic and Interventional Imaging*, Société française de radiologie, pp. 3–5.
- 22 20 Singh, S., Prakash, C. and Ramakrishna, S. (2019), “3D printing of polyether-ether-ketone
23 21 for biomedical applications”, *European Polymer Journal*, Elsevier, Vol. 114 No.
24 22 February, pp. 234–248.
- 25 23 Sobaszek, A., Hache, J.C., Frimat, P., Akakpo, V., Victoire, G. and Furon, D. (1999),
26 24 “Working conditions and health effects of ethylene oxide exposure at hospital
27 25 sterilization sites.”, *Journal of Occupational and Environmental Medicine*, United States,
28 26 Vol. 41 No. 6, pp. 492–499.
- 29 27 Sowah, R.A. and Ahiabor, C. (2014), “Effectiveness of UV Sterilisation Chambers in
30 28 Barbering Shops and Salons”, *Journal of Natural Sciences Research*, Vol. 4, pp. 67–74.
- 31 29 Tipnis, N.P. and Burgess, D.J. (2018), “Sterilization of implantable polymer-based medical
32 30 devices: A review”, *International Journal of Pharmaceutics*, Elsevier B.V., Vol. 544 No.
33 31 2, pp. 455–460.
- 34 32 Vasamsetty, P., Pss, T., Kukkala, D., Singamshetty, M. and Gajula, S. (2020), “3D printing in
35 33 dentistry – Exploring the new horizons”, *Materials Today: Proceedings*, available
36 34 at:<https://doi.org/https://doi.org/10.1016/j.matpr.2020.01.049>.
- 37 35 Wesemann, C., Pieralli, S., Fretwurst, T., Nold, J., Nelson, K., Schmelzeisen, R., Hellwig, E.,
38 36 *et al.* (2020), “3-D Printed Protective Equipment During COVID-19 Pandemic”,
39 37 *Materials*, Vol. 13 No. 8, p. 1997.
- 40 38 Yang, H., Wang, B. and Ma, L. (2019), “Mechanical properties of 3D double-U auxetic
41 39 structures”, *International Journal of Solids and Structures*, Vol. 180–181, pp. 13–29.
- 42 40 Yoganarasimha, S., Best, A. and Madurantakam, P.A. (2019), “Peracetic acid sterilization
43 41 induces divergent biological response in polymeric tissue engineering scaffolds”,
44 42 *Applied Sciences (Switzerland)*, Vol. 9 No. 18, pp. 1–12.
- 45 43 Zhao, Y., Zhu, B., Wang, Y., Liu, C. and Shen, C. (2019), “Effect of different sterilization
46 44 methods on the properties of commercial biodegradable polyesters for single-use,
47 45 disposable medical devices”, *Materials Science and Engineering C*, Elsevier, Vol. 105
48 46 No. March, p. 110041.
- 49 47 Zhu, S., Ruiz de Azua, I.V., Feijen, S., van der Goot, A.J., Schutyser, M. and Stieger, M.
50 48 (2021), “How macroscopic structure of 3D printed protein bars filled with chocolate
51 49 influences instrumental and sensory texture”, *Lwt*, Elsevier Ltd, Vol. 151 No. May, p.
52 50 112155.
53
54
55
56
57
58
59
60


Table 1. 3D printing parameters

No.	Selected parameters	Value
1.	Nozzle temperature	200°C
2.	Bed temperature	65°C
3.	Nozzle diameter	0.4 mm
4.	Filament diameter	1.75 mm
5.	Layer thickness	0.1 mm
6.	Fiber orientation to specimen axis	+45°/-45°
7.	Outline	2
8.	Top/bottom solid layers	6/6

Table. 2. Calculated values of tensile strength parameters


PLA part	Ultimate Tensile Strength, σ_M , MPa		Young modulus, E , MPa		Toughness, Q , MJ/m ³	
	Mean \pm STD	Median	Mean \pm STD	Median	Mean \pm STD	Median
Non-sterilised	57.92 \pm 0.66	58.22	3585.45 \pm 123.32	3598.36	1.007 \pm 0.004	1.021
UV light-sterilised	53.38 \pm 0.16	53.37	3116.28 \pm 195.01	3045.35	1.080 \pm 0.060	1.049
EtO-sterilised	55.54 \pm 0.47	55.55	3121.81 \pm 216.14	3121.92	1.059 \pm 0.090	1.040

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

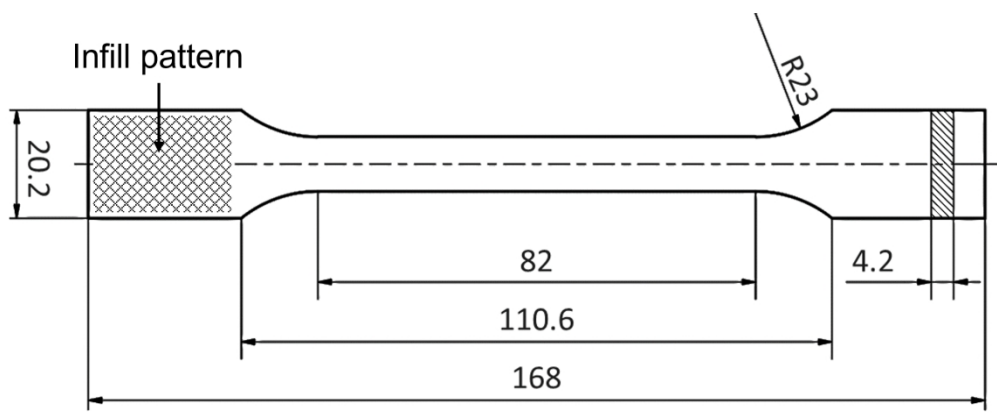

Geometry of dog-bone shaped specimen.


485x196mm (130 x 130 DPI)

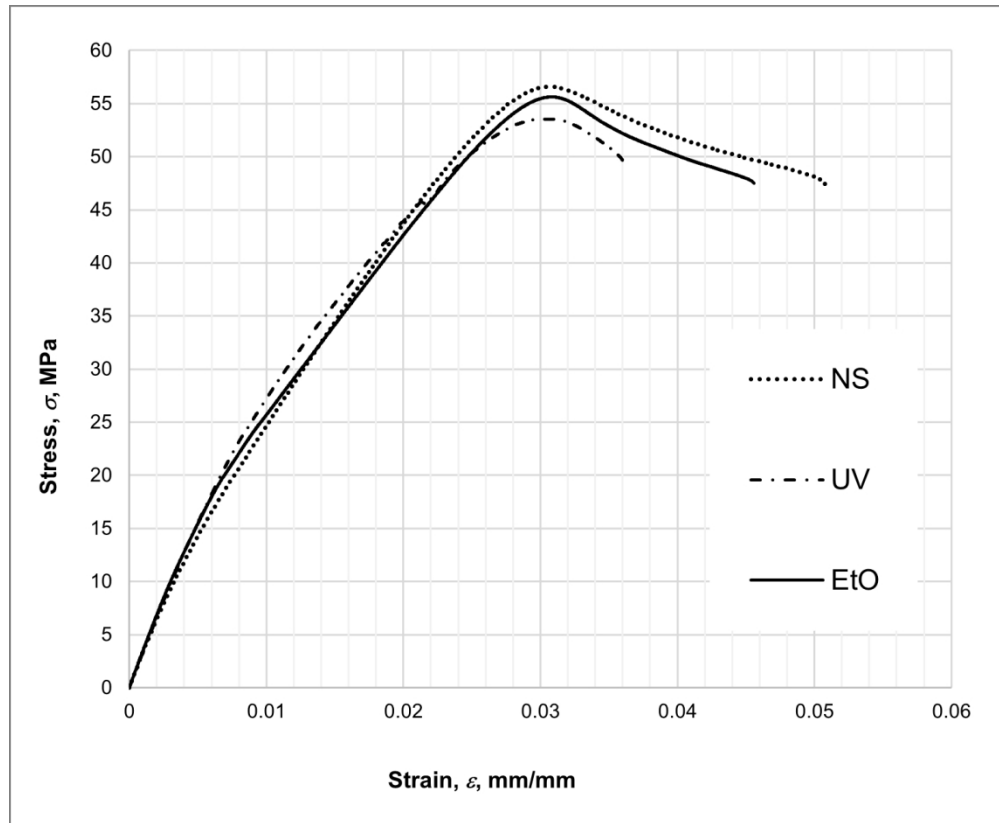

The representative stress–strain curves of the specimens before (NS) and after UV light or EtO sterilization.


314x257mm (130 x 130 DPI)

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

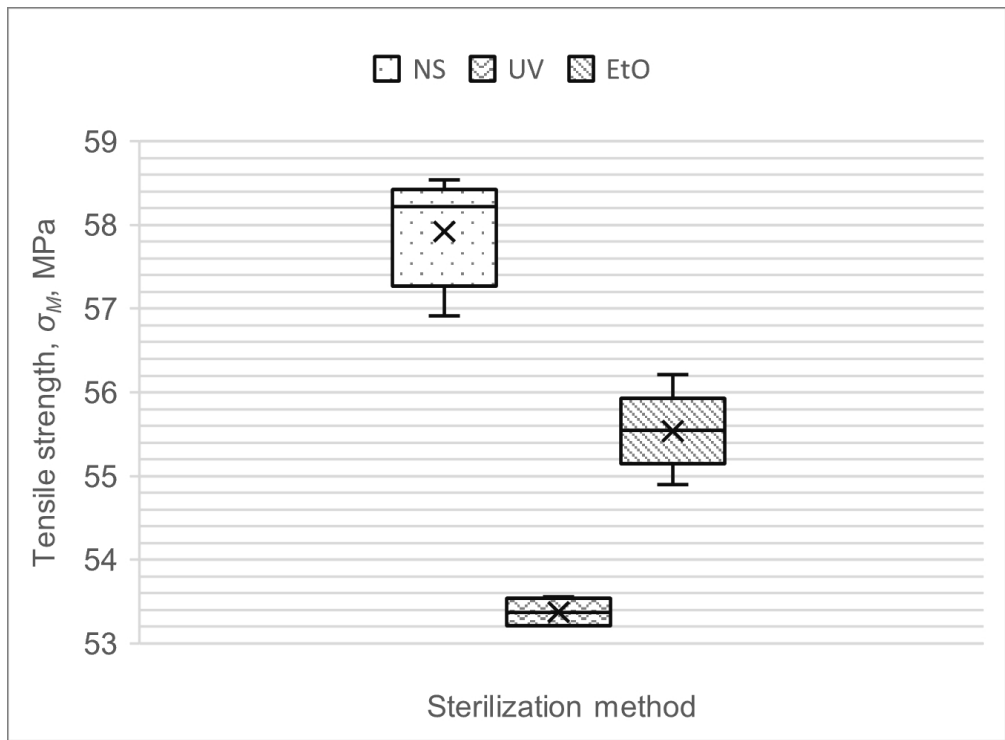

Comparison of mechanical properties: a) tensile strength, b) Young modulus, c) toughness.


263x193mm (130 x 130 DPI)

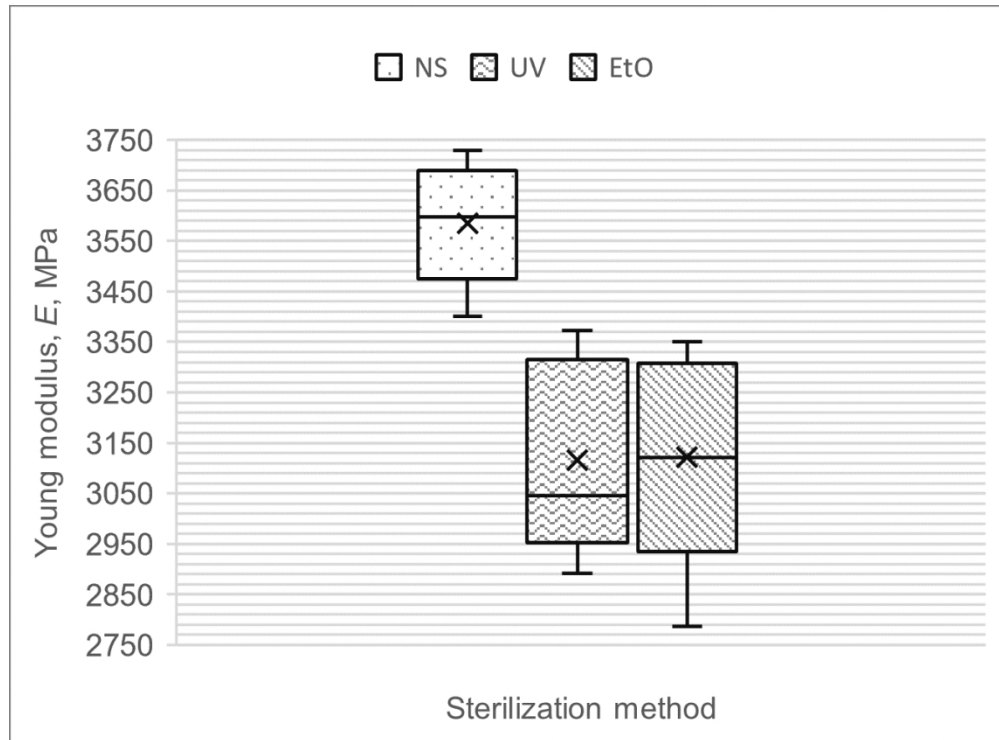

Comparison of mechanical properties: a) tensile strength, b) Young modulus, c) toughness.

262x193mm (130 x 130 DPI)

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

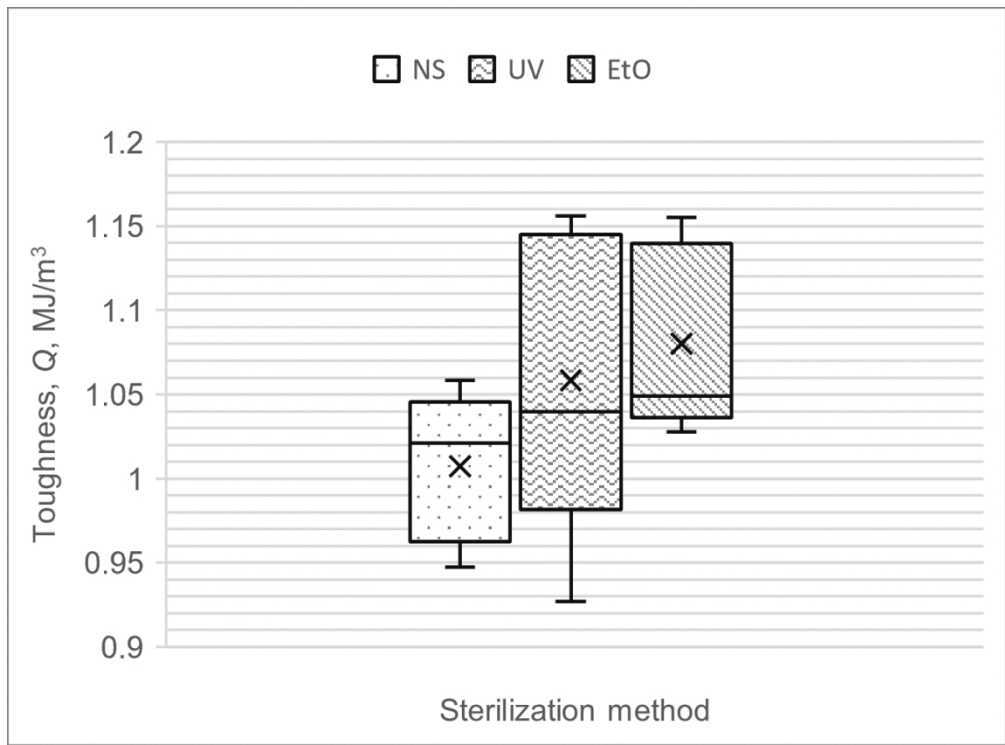

Comparison of mechanical properties: a) tensile strength, b) Young modulus, c) toughness.

262x193mm (130 x 130 DPI)