



$l_{ua}$  – upper respiratory tract inertance [ $\text{cmH}_2\text{O}^2 \cdot \text{s} \cdot \text{l}^{-1}$ ],  $l_c$  – central respiratory tract inertance [ $\text{cmH}_2\text{O}^2 \cdot \text{s} \cdot \text{l}^{-1}$ ],  $l_t$  – thoracic wall inertance [ $\text{cmH}_2\text{O}^2 \cdot \text{s} \cdot \text{l}^{-1}$ ],  $C_{gua}$  – oral cavity gas compliance [ $\text{cmH}_2\text{O}^{-1} \cdot \text{l}$ ],  $C_{uaw}$  – upper respiratory tract walls compliance [ $\text{cmH}_2\text{O}^{-1} \cdot \text{l}$ ],  $C_{aw}$  – bronchial walls compliance [ $\text{cmH}_2\text{O}^{-1} \cdot \text{l}$ ],  $C_g$  – alveoli gas compliance [ $\text{cmH}_2\text{O}^{-1} \cdot \text{l}$ ],  $C_i$  – lung tissue compliance [ $\text{cmH}_2\text{O}^{-1} \cdot \text{l}$ ],  $C_t$  – thoracic wall compliance [ $\text{cmH}_2\text{O}^{-1} \cdot \text{l}$ ],  $P_g$  – variable breathing cycle pressure [ $\text{cmH}_2\text{O}$ ],  $P_t$  – thorax tissue tension [ $\text{cmH}_2\text{O}$ ],  $P_{ao}$  – respiratory tract outlet pressure [ $\text{cmH}_2\text{O}$ ],  $dV_{ao}/dt$  – respiratory tract outlet flow [ $\text{l/s}$ ]

**Rys. 1.** Model układu oddechowego człowieka zamodelowany w aplikacji [15]:

$R_{uaw}$  – oporność ścian górnych dróg oddechowych [ $\text{cmH}_2\text{O} \cdot \text{s} \cdot \text{l}^{-1}$ ],  $R_{ua}$  – oporność górnych dróg oddechowych [ $\text{cmH}_2\text{O} \cdot \text{s} \cdot \text{l}^{-1}$ ],  $R_c$  – oporność centralnych dróg oddechowych [ $\text{cmH}_2\text{O} \cdot \text{s} \cdot \text{l}^{-1}$ ],  $R_p$  – oporność peryferyjnych dróg oddechowych [ $\text{cmH}_2\text{O} \cdot \text{s} \cdot \text{l}^{-1}$ ],  $R_l$  – oporność tkanek płuc [ $\text{cmH}_2\text{O} \cdot \text{s} \cdot \text{l}^{-1}$ ],  $R_t$  – oporność ścian klatki piersiowej [ $\text{cmH}_2\text{O} \cdot \text{s} \cdot \text{l}^{-1}$ ],  $l_{uaw}$  – inertancja ścian górnych dróg oddechowych [ $\text{cmH}_2\text{O}^2 \cdot \text{s} \cdot \text{l}^{-1}$ ],  $l_{ua}$  – inertancja górnych dróg oddechowych [ $\text{cmH}_2\text{O}^2 \cdot \text{s} \cdot \text{l}^{-1}$ ],  $l_c$  – inertancja centralnych dróg oddechowych [ $\text{cmH}_2\text{O}^2 \cdot \text{s} \cdot \text{l}^{-1}$ ],  $l_t$  – inertancja ścian klatki piersiowej [ $\text{cmH}_2\text{O}^2 \cdot \text{s} \cdot \text{l}^{-1}$ ],  $C_{gua}$  – podatność gazu w jamie ustnej [ $\text{cmH}_2\text{O}^{-1} \cdot \text{l}$ ],  $C_{uaw}$  – podatność ścian górnych dróg oddechowych [ $\text{cmH}_2\text{O}^{-1} \cdot \text{l}$ ],  $C_{aw}$  – podatność ścian oskrzeli [ $\text{cmH}_2\text{O}^{-1} \cdot \text{l}$ ],  $C_g$  – podatność gazu pęcherzyków płucnych [ $\text{cmH}_2\text{O}^{-1} \cdot \text{l}$ ],  $C_i$  – podatność tkanek płuc [ $\text{cmH}_2\text{O}^{-1} \cdot \text{l}$ ],  $C_t$  – podatność ścian klatki piersiowej [ $\text{cmH}_2\text{O}^{-1} \cdot \text{l}$ ],  $P_g$  – zmienne ciśnienie cyklu oddechowego [ $\text{cmH}_2\text{O}$ ],  $P_t$  – napięcie tkanek klatki piersiowej [ $\text{cmH}_2\text{O}$ ],  $P_{ao}$  – ciśnienie u wylotu dróg oddechowych [ $\text{cmH}_2\text{O}$ ],  $dV_{ao}/dt$  – przepływ u wylotu dróg oddechowych [ $\text{l/s}$ ]

The last step of the modeling is to analyze physiological changes caused by asthma. To achieve this, a modification of the model parameters shown in fig. 1 was proposed. The modified parameters will be used to test the, proposed for educational purposes, application. Asthma is a disease that causes airway obstruction over their entire length. Bronchial obstruction, causes a change of their resistance and inertance. According to [10–11], the change in resistance is proportional to the fourth power of the bronchi radius (assuming laminar flow), whereas inertance – the square of the radius. Based on a review of the literature [10, 12–13], changes in the parameters of the model in fig. 1 were made, which are shown in tab. 1.

**Tab. 1.** The values of physical parameters representing the patient's considered health statuses


**Tab. 1.** Wartości wielkości fizycznych reprezentujących rozpatrywane stany zdrowia pacjenta

The examined patient's state	Central airways		Distal airways
Healthy	$R_c$	$I_c$	$R_p$
Asthma case 1	$5 R_c$	$2 I_c$	$5 R_p$
Asthma case 2	$2.5 R_c$	$1.5 I_c$	$2.5 R_p$

### 3. Control layer

The Control Layer of educational application was created with LabVIEW environment of National Instruments Corporation and its user panel is illustrated in fig. 3. It consists of a control panel, on which all the changes in the physical parameters  $R_c$ ,  $I_c$  oraz  $R_p$  are made. These changes result in modifications to the mechanics of the respiratory system, which are presented in charts. Mechanics examination is made with the use of the forced oscillation method (Forced Oscillation Technique, FOT). This method has been described in many publications, e.g. [14–17] and has gained wide acceptance and recognition because of the high sensitivity and the effectiveness of detection of early flow limitation phenomenon [15, 17]. FOT algorithm is illustrated in fig. 2. The essence of FOT is to provide the pressure wave  $P(t)$ , containing one or several frequencies, at the patient's mouth. Amplitude of the pressure wave  $A$  can be changed with the knob located on the control panel. As a result of these actions, the primary breathing waveforms of pressure  $P_{ao}(t)$  and flow  $dV_{ao}(t)/dt$  are modified to a form including higher harmonics. The measurement data of the resulting pressure wave  $P_{aof}(t)$  and flow  $dV_{aof}(t)/dt$  is then subjected to sampling and Fourier transformation. Course of lung impedance in frequency domain is obtained by dividing the result pressure and frequency data (fig. 2).

The result of the application calculations are the waveforms of the real and imaginary impedance  $Z(f)$ . Those waveforms, obtained with frequency methods, can be then used for purposes of educational analyses. As a complement to the results of lung mechanics, both pressure and flow time courses with the oral cavity reference (fig. 1) are displayed.

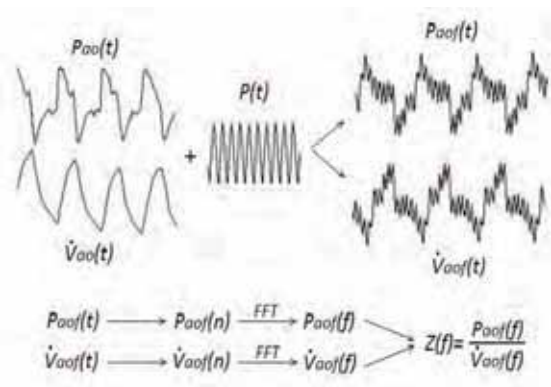


**Fig. 2.** Algorithm of FOT method based on [18]

**Rys. 2.** Algorytm metody FOT [18]

Control layer was connected with the MATLAB/Simulink respiratory system model through Simulation Interface Toolkit. It is contained into the set of libraries of the LabVIEW environment and its task is to establish a virtual data server, used by the connected applications. Moreover, the user has the ability to save the results of frequency analysis in the form of a text file and, if he has a need, upload up to two frequency courses stored previously. That data will be plotted along with the currently analyzed results.


#### 4. The results of diagnostic tests for the considered diseases

The model presented in fig. 1 has been subjected to portray the application's diagnostic process and its results. In order to map the healthy human respiratory system mechanics (tab. 1), necessary changes of model's parameter values have been made with instruments placed on the control panel. The simulation results with the visualization of the time course of pressure, or flow rate with the oral cavity reference in real time. Then, after a few seconds of the measurement, the application starts the calculation process of pulmonary mechanics according to fig. 2. Figure 3 illustrates the results of calculations of the healthy patient respiratory system mechanics, complemented with airflow time course with the oral cavity reference. In order to model respiratory mechanics changes, caused by asthma, physical parameters  $R_c$ ,  $I_c$  and  $R_p$  have been changed (according to the tab. 1). For both settings cases (of asthma 1 and asthma 2), all actions described for a healthy individual model were repeated. The diagnostic results of all three individuals were archived for collective visualization, which is illustrated in fig. 4.

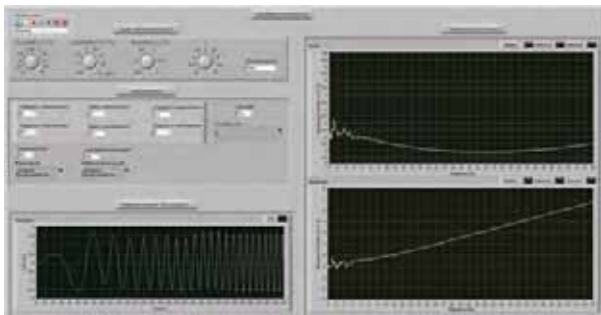

**Fig. 3.** User's application panel view with results of the simulation performed for a clinical case of a healthy individual

**Rys. 3.** Widok na panel użytkownika aplikacji wyraz z wynikami symulacji prowadzonej dla przypadku pacjenta zdrowego

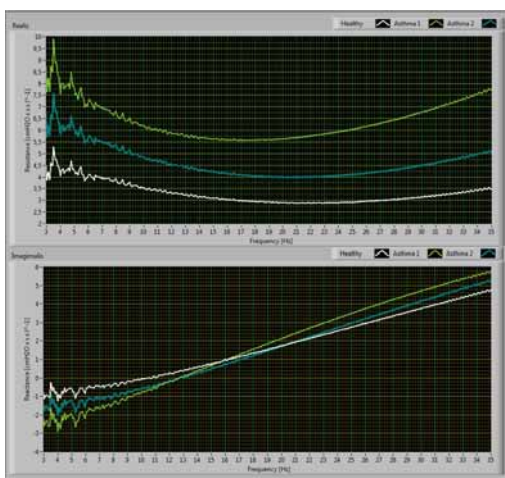

**Fig. 4.** Graphical results of the simulation performed for three clinical cases of various patient's health condition

**Rys. 4.** Wyniki symulacji przeprowadzonej dla trzech przypadków stanu zdrowia pacjenta

#### 5. Summary and conclusions

In conclusion, designing and developing comprehensive educational applications in the field of bioengineering, can be used in both raising social awareness and improving the teaching and learning processes at all levels of education of the professionals (engineers, masters, doctors, etc.). Examples of such applications can be found in the literature [19–20]. In the future, these types of systems can also provide a foundation for intelligent systems supporting medical diagnosing and treatment. Application presented in this paper is undoubtedly a proposal of medical tool, streamlining the teaching process of detecting obstructive diseases of the human respiratory system. However, the structure of a presented educational platform allows its developers to use it in problem-oriented tasks, and in numerous and widely used e-learning systems.

#### References

1. Lehnen J., Panaszek B., Pluta J., Bohater P., *Choroby dróg oddechowych*, MedPharm, Wrocław 2011.
2. Massaro D., Massaro G., *Estrogen regulates pulmonary alveolar formation, loss, and regeneration in mice*, "American Journal of Physiology Lung Cellular and Molecular Physiology", 6/2004, L1154–L1159.
3. Officer T., Pellegrino M., Brusasco V., Rodarte J., *Measurement of pulmonary resistance and dynamic compliance with airway obstruction*, "Journal of Applied Physiology", 5/1998, 1982–1988.
4. Piwowar P., *Pomiar mechanicznych parametrów dróg oddechowych metodą wymuszania krótkotrwałych, ujemnych impulsów ciśnienia*, Rozprawa doktorska, Akademia Górniczo-Hutnicza, Kraków 2006.
5. Piwowar P., *Diagnosing human's airduct disease by negative pressure impulse method*, Proceedings of the 23<sup>rd</sup> IEEE Instrumentation and Measurement Technology Conference, Sorrento, Italy, 2006.
6. Peslin R., *Computer simulation of respiratory impedance and flow transfer functions during high frequency oscillations*, "British Journal of Anaesthesiology", 7/1989, 91–94.
7. Rotger M., Peslin R., Duvivier C., Navajas D., Gallina C., *Density dependence of respiratory input and transfer impedances in humans*, "Journal of Applied Physiology", 2/1988, 928–933.
8. Cauberghe M., Van de Woestijne K., *Mechanical properties of the upper airway*, "Journal of Applied Physiology", 2/1983, 335–342.
9. Peslin R., Duvivier C., Jardin P., *Upper airway walls impedance measured with head plethysmograph*, "Journal of Applied Physiology", 2/1984, 596–600.
10. Ritz T. et al, *Special report. Guidelines for mechanical lung function measurements in psychophysiology*, "Psychophysiology", 5/2002, 546–567.
11. Carvalho A., Zin W., *Respiratory Mechanics: Principles, Utility and Advances*, [in:] Gullo A.,

„Anaesthesia, Pharmacology, Intensive Care and Emergency Medicine A.P.I.C.E.”, Springer Milan, Milan 2011.

12. Weinberger S. E., Cockrill B. A., Mandel J., *Principles of Pulmonary Medicine 5e*, Saunders Elsevier, Philadelphia 2008.
13. Rajagiri A., Diong B., Goldman M., Nazeran H., *Can Asthma in Children be Detected by the Estimated Parameter Values of the Augmented RIC Model?*, Proceedings of the 28<sup>th</sup> IEEE EMBS Annual International Conference, New York City, USA, 2006.
14. DuBois A. B., Brody A.W., Levis D. H., Burgess B. F., *Oscillation mechanics of the lung and chest in humans*, “Journal of Applied Physiology”, 8/1956, 587–594.
15. Dellaca R.L. et al, *Expiratory flow limitation detected by forced oscillation and negative expiratory pressure*, “European Respiratory Journal”, 2/2007, 363–374.
16. Faria A. et al, *Forced oscillation technique in the detection of smoking-induced respiratory alterations: diagnostic accuracy and comparison with spirometry*, “CLINICS”, 12/2010, 1295–1304.
17. [http://www.biomedical-engineering-online.com/content/8/1/22] – Faria A. et al, *Evaluating the forced oscillation technique in the detection of early smoking-induced respiratory changes*, “BioMedical Engineering OnLine”, 8/2009.
18. Tadeusiewicz R., Augustyniak P., *Podstawy inżynierii biomedycznej*, Wydawnictwa AGH, Kraków 2009.
19. Izvorski A., Koleszyńska J., Tadeusiewicz R., Bulka J., Wochlik I., *GIGISIM (Glucose-Insulin and Glycemic Index Web Simulator) – the online system supporting diabetes therapy*, The IASTED International Conference on Telehealth ACTA Press Calgary, Canada, 2005.
20. Lehmann E. D., *Interactive educational simulators in diabetes care*, “International Journal of Medical Informatics”, 1/1997, 47–76. ■

### **Aplikacja wspomagająca procesy edukacyjne w zakresie wykrywania chorób obturacyjnych układu oddechowego**

**Streszczenie:** W publikacji zaprezentowano działanie platformy wspomagającej edukację w zakresie wykrywania chorób obturacyjnych układu oddechowego. Rolę badanego pacjenta pełni 16-elementowy model układu oddechowego, symulowany w środowisku MATLAB/Simulink. Został on połączony z warstwą sterowania, wykonaną w środowisku LabVIEW, przy pomocy biblioteki SIT (Simulation Interface Toolkit).

Warstwa ta odpowiada za modyfikację parametrów modelu oraz generowanie wyników pomiaru impedancji układu oddechowego za pomocą oscylacji wymuszonych. Wykonana aplikacja jest rozwiązaniem zapewniającym dużą elastyczność w kształceniu studentów związanych z inżynierią biomedyczną i naukami o zdrowiu i bardzo łatwo może być wdrożona do pracy jako rozwiązanie e-learningowe, zorientowane problemowo.

**Słowa kluczowe:** aplikacja komputerowa, choroby obturacyjne, płuca

---

#### **Grzegorz Redlarski, PhD DSc Eng**

Headmaster of the Department of Mechatronics and High Voltage Engineering at the Electrical and Control Engineering Faculty at Gdańsk University of Technology. He received his M.Sc. in 2000 within the specialization of control engineering and advanced in the specialization of electrical engineering. As a result, he received his PhD in 2003 and DSc in 2011. From 2011 he is also employed as a Associate Professor at the Faculty of Technical Sciences at the University of Warmia and Mazury in Olsztyn. His main fields of interest are power electronics, power engineering and, recently, biomedical engineering.

*e-mail: g.redlarski@ely.pg.gda.pl*



#### **Jacek Jaworski, MSc Eng**

Lecturer in the Department of Mechatronics and High Voltage Engineering at the Electrical and Control Engineering Faculty at Gdansk University of Technology. He received his MSc in 2011 in the major of Control Engineering and Robotics, specialization Control Engineering. Main fields of interests are: biomedical engineering and application of control and signal processing systems in medical sciences.

*e-mail: jjaworski@ely.pg.gda.pl*



#### **Piotr Mateusz Tojza, MSc Eng**

Lecturer in the Department of Mechatronics and High Voltage Engineering at the Electrical and Control Engineering Faculty at Gdańsk University of Technology. He received his MSc in 2011 in the major of Control Engineering and Robotics, specialization Robotics and Mechatronic Systems. His main fields of interests are: biomedical engineering and application of robotics and mechatronics systems in medical sciences.

*e-mail: ptojza@ely.pg.gda.pl*

